UNIVERSITY OF HOUSTON
Learning. Leading.

MEDIPIX: A Technology Developed at CERN, That Can Be Developed As An Active Real-time Space Radiation Dosimeter

Lawrence Pinsky

University of Houston

Note that Michael Campbell, CERN

(The Medipix2 Consortium Spokesperson)

Is Also Present at this meeting…

Important Disclaimers

- Note that ALL DISCLOSURES regarding the Design and Performance of the MEDIPIX technology made in this presentation is to be considered CONFIDENTIAL to the extent that subsequent patent applications may be submitted.
- The University of Houston is NOT presently a member of the Medipix Consortium, but rather we have been formally invited by that Collaboration to join for the purpose of pursuing the adaptation of this technology to Space Radiation Dosimetry…

The Medipix2 Consortium

- Institut de Fisca d'Altes Energies, Barcelona, Spain
- University of Cagliari and INFN Section thereof, Italy
- CEA, Paris, France
- CERN, Geneva, Switzerland,
- Universitat Freiburg, Freiburg, Germany,
- University of Glasgow, Scotland
- Universita' di Napoli and INFN Section thereof, Italy
- NIKHEF, Amsterdam, The Netherlands
- University of Pisa and INFN Section thereof, Italy
- University of Auvergne, Clermont Ferrand, France,
- Laboratory of Molecular Biology, Cambridge England
- Mitthogskolan, Sundsvall, Sweden,
- Czech Technical University, Prague, Czech Republic
- ESRF, Grenoble, France
- Academy of Sciences of the Czech Republic, Prague
- Universität Erlangen-Nurnberg, Erlangen, Germany
- University of California-SSL, Berkeley, USA

WHAT IS MEDIPIX2 DETECTOR?

Medipix2 is a pixel-based detector technology that can be employed to measure charged particles, photons (visible through gammas), and neutrons. It is based on a read-out chip that embeds the electronics for each pixel within the pixel's footprint!

Outline of This Talk

- The Medipix2 Chip and Readout System
- Recent Heavy Ion Beam Medipix Exposures
- Timepix—An Evolution Within Medipix2
- Medipix3—The Next Generation of Medipix
- Where Do We Go From Here With Medipix

Hybrid Pixel Detector

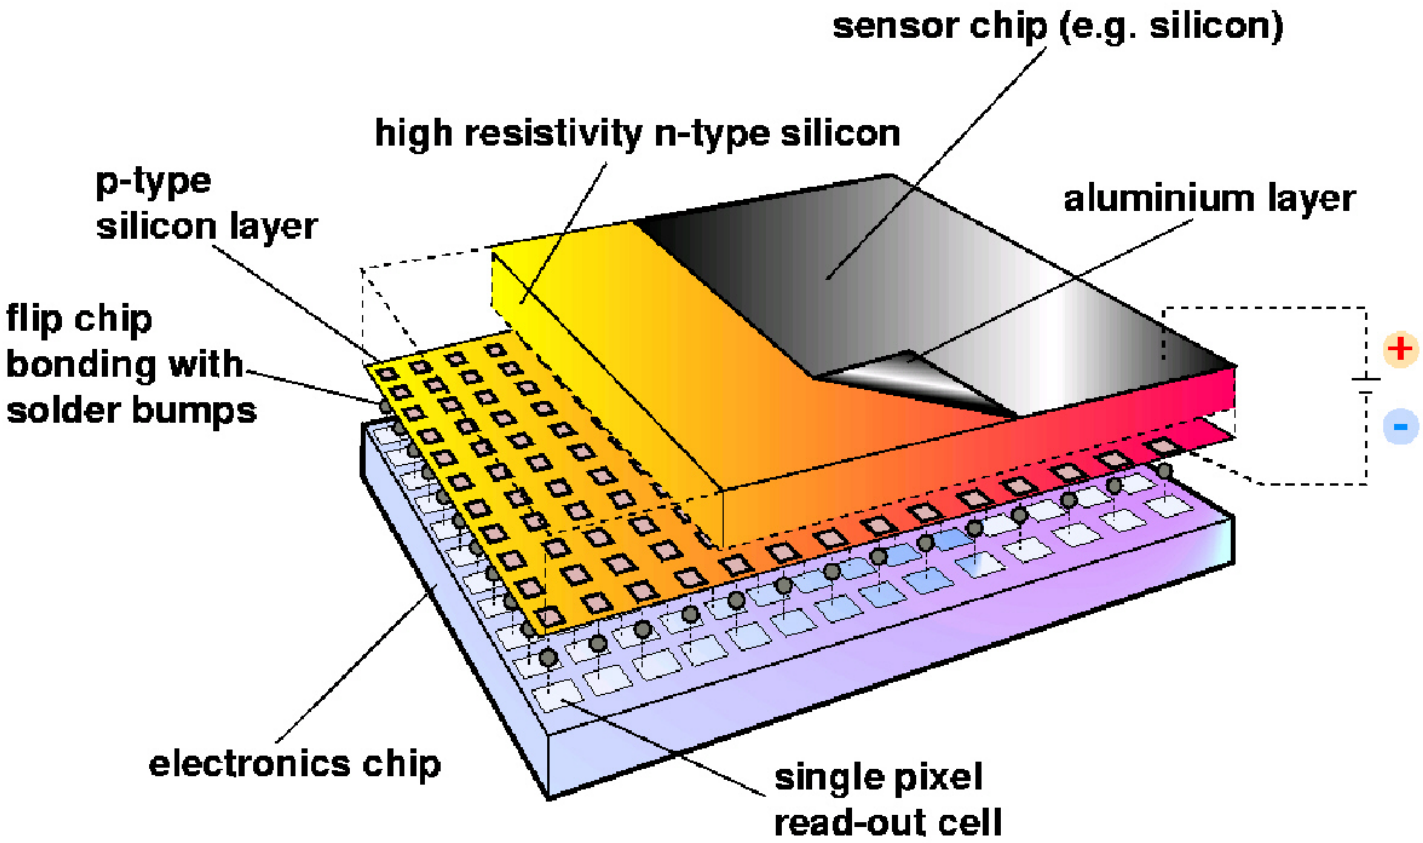

Detector and electronics readout are optimized separately

Hybrid Pixel Detector - Cross Section

Current Medipix2 Cell Schematic

Charge sensitive preamplifier with individual leakage current compensation
2 discriminators with globally adjustable thresholds
3-bit local fine tuning of the threshold per discriminator
1 test and1 mask bit
External shutter activates the counter
13-bit pseudo-random counter
1 Overflow bit

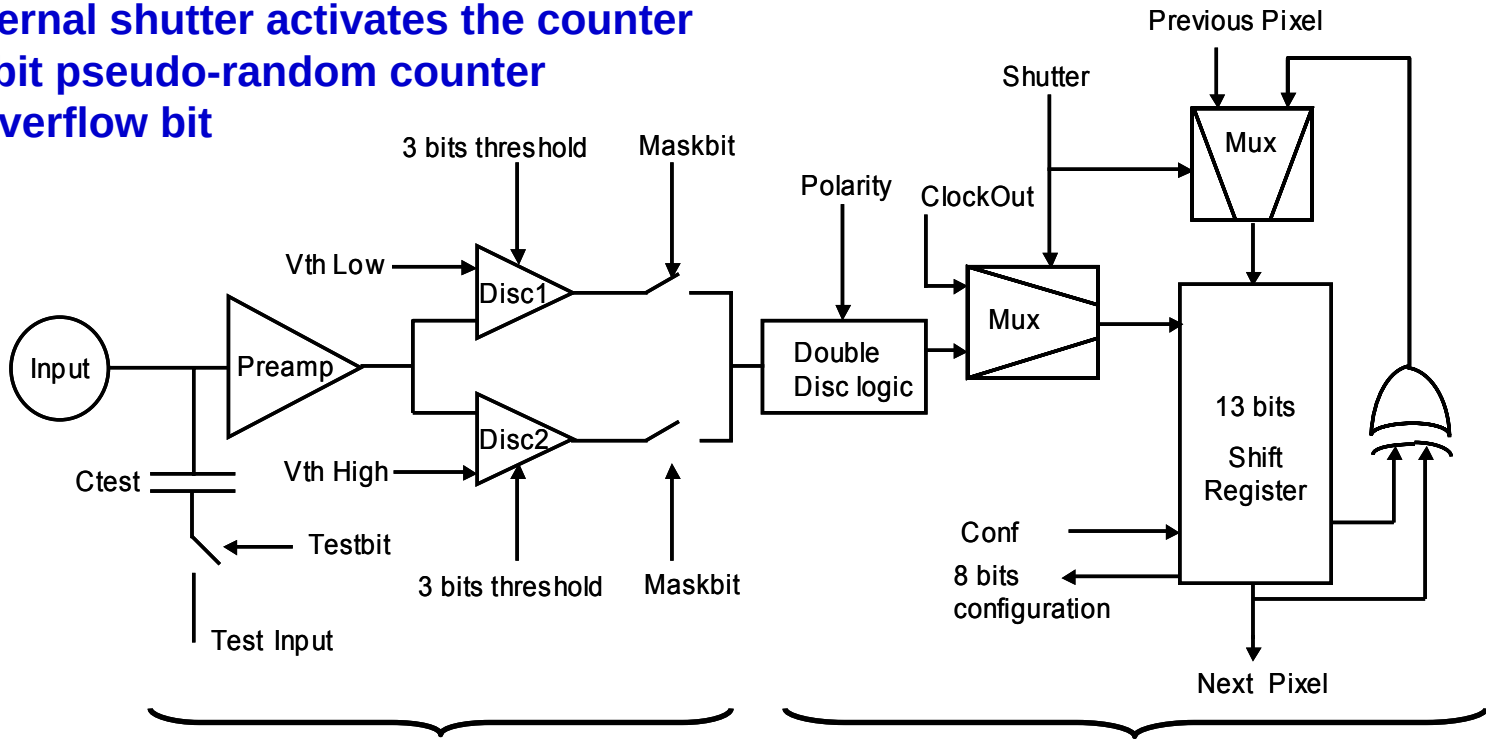

Current Medipix2 Cell Layout

503 transistors per pixel

33M per Chip

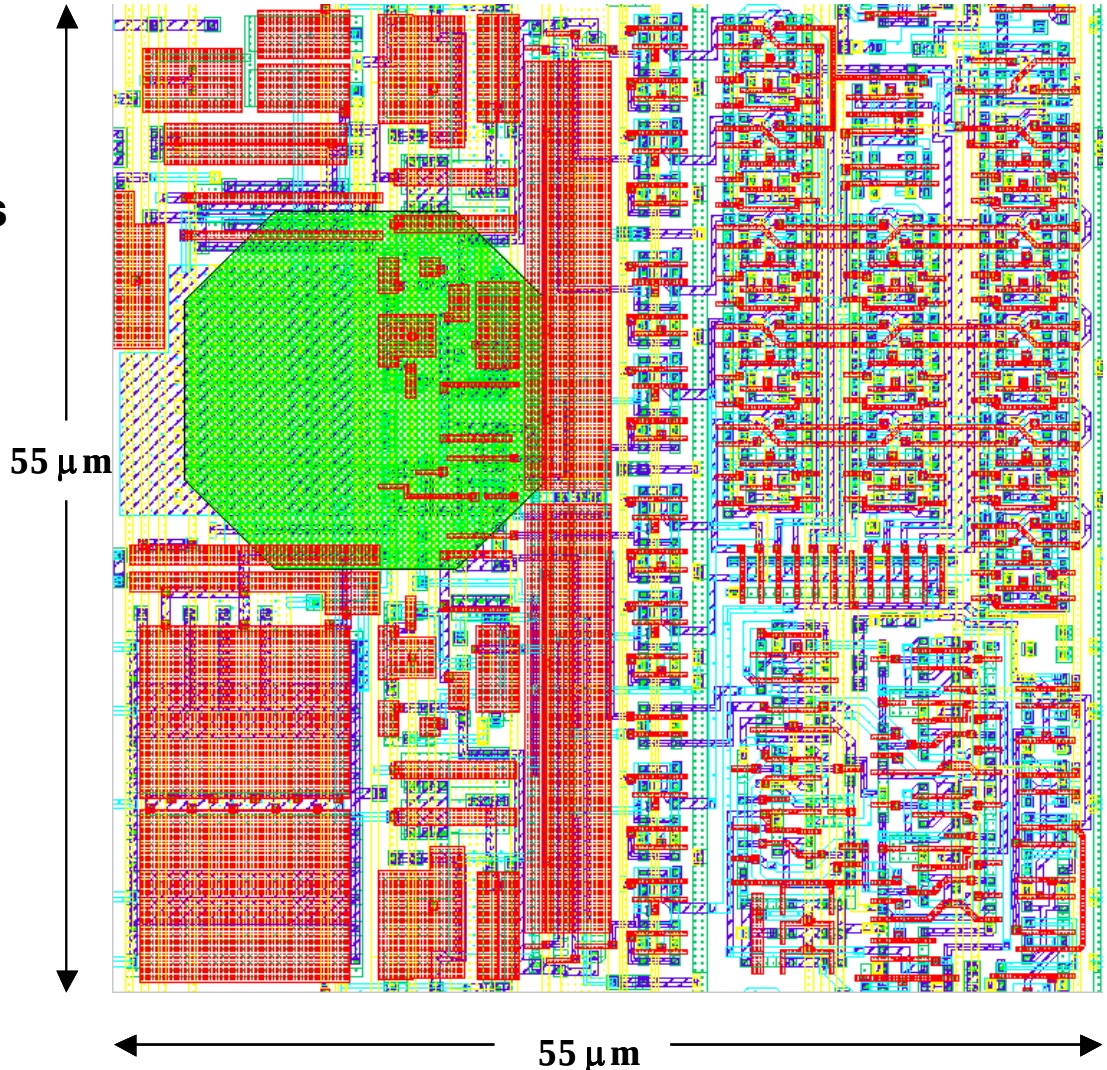

Bumps on the readout side

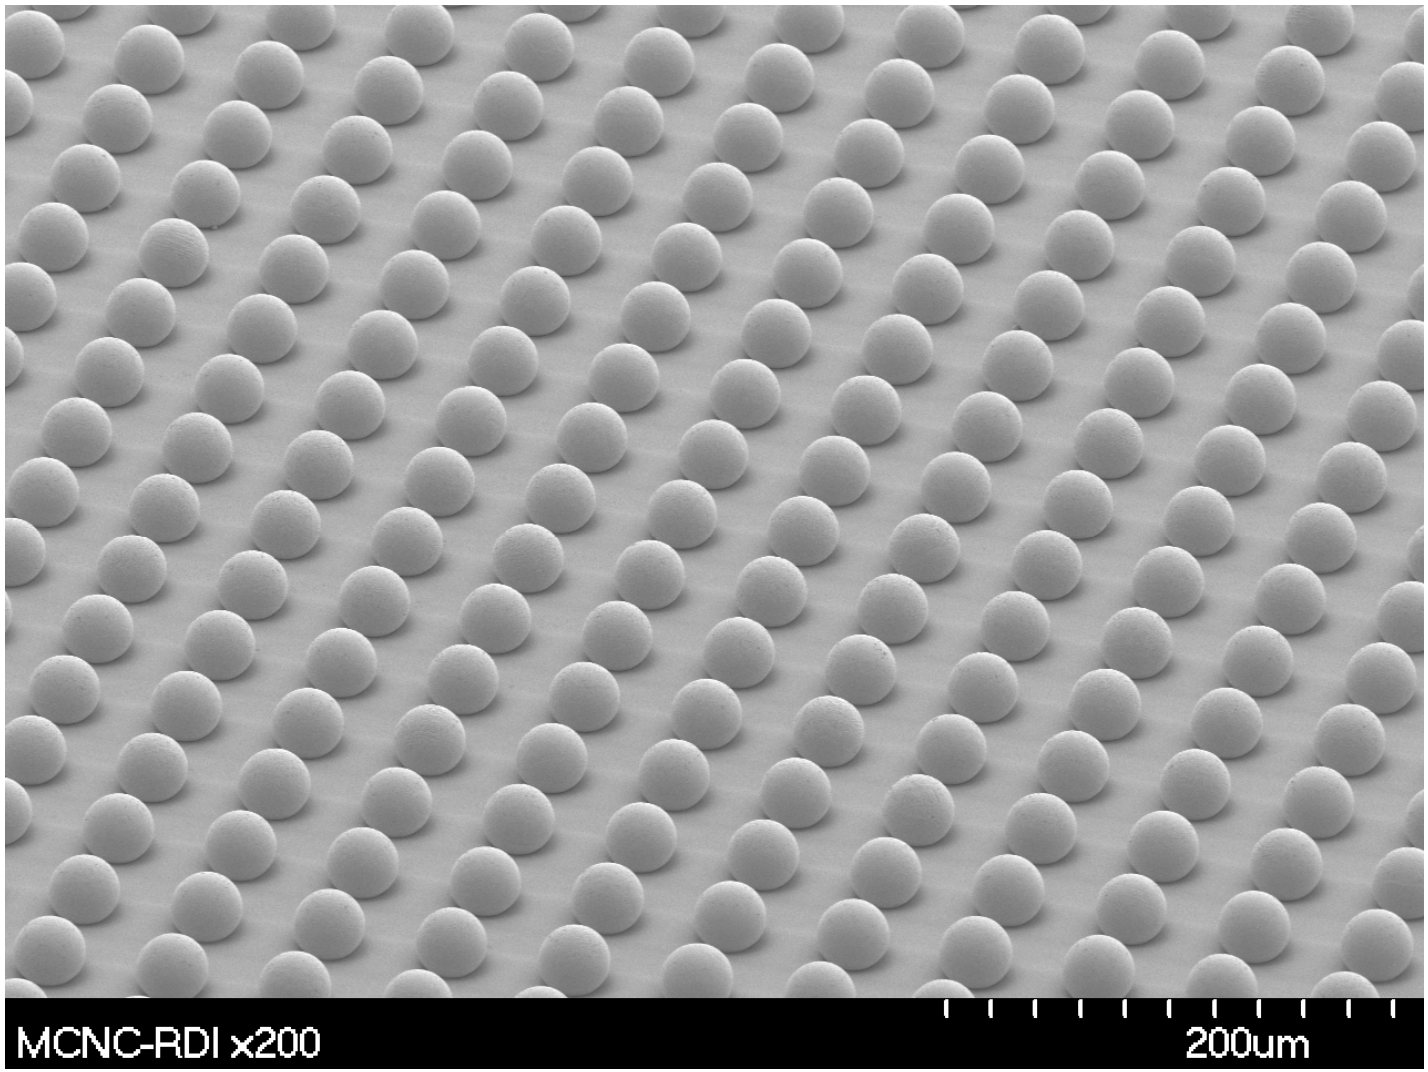

Bumps on the readout side – close up

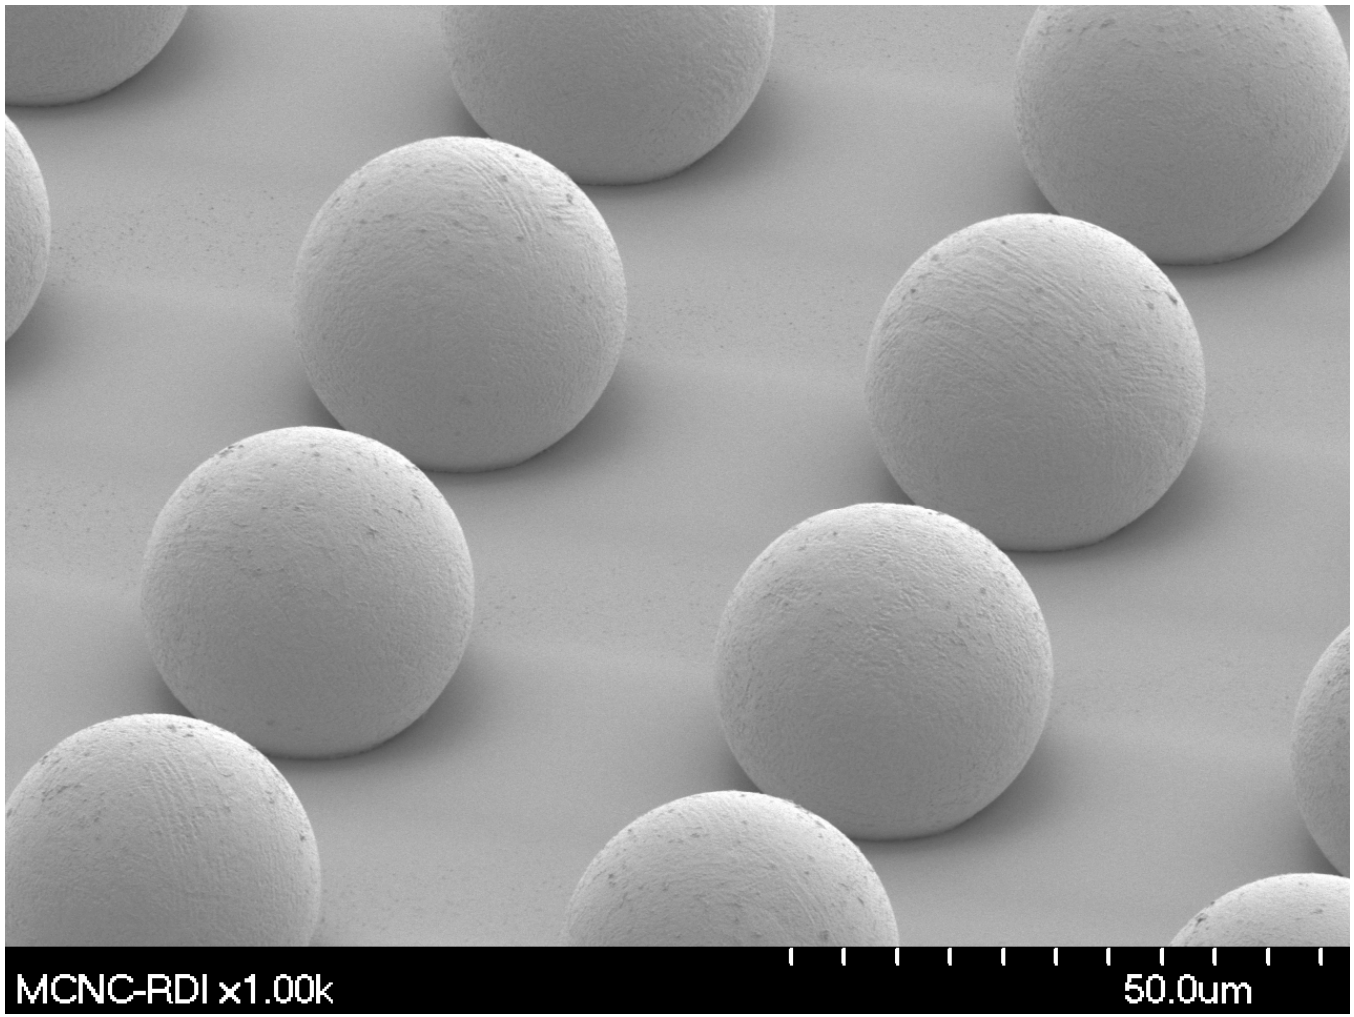

Medipix2 Si Assembly

A new USB based Medipix2 Readout System

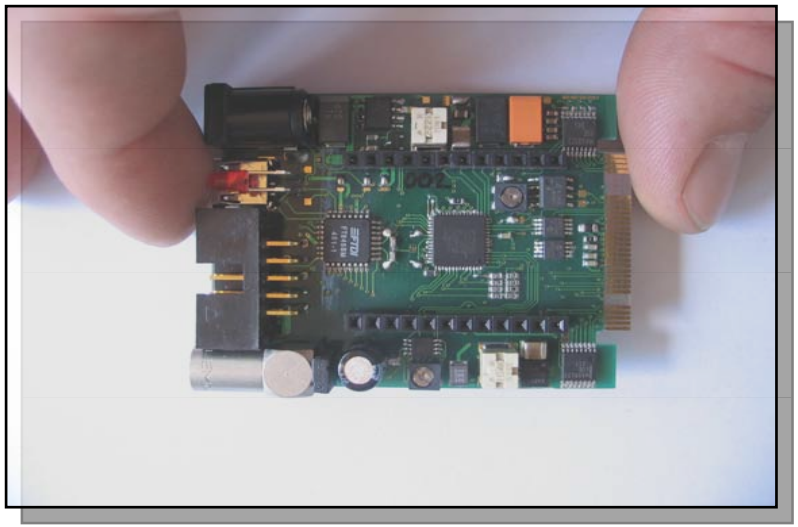

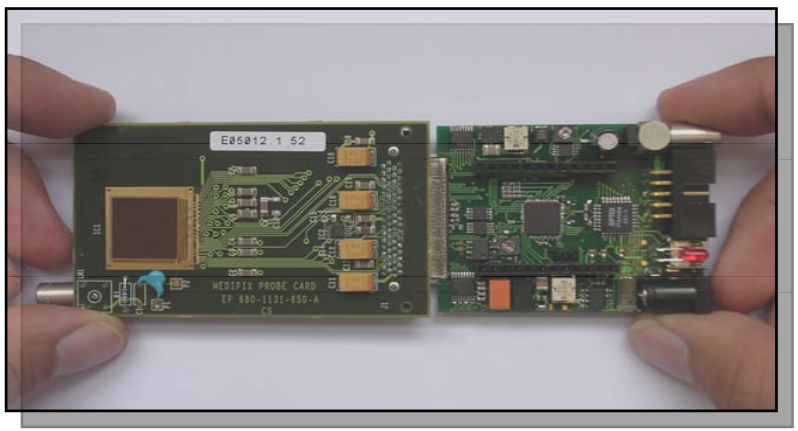

USB1 compatible
Developed by S. Pospisil et al.
CTU, Prague

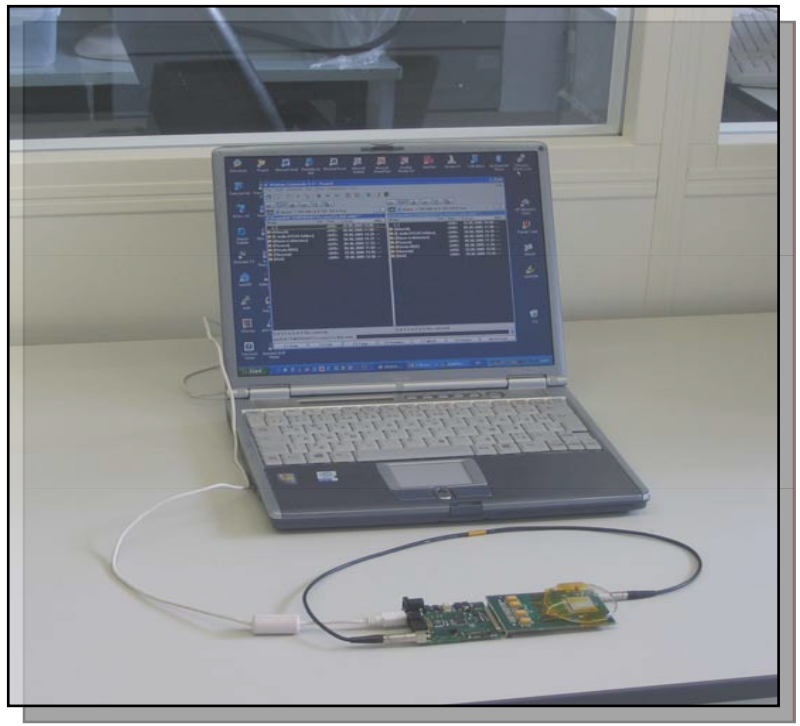

Image of a dried anchovy

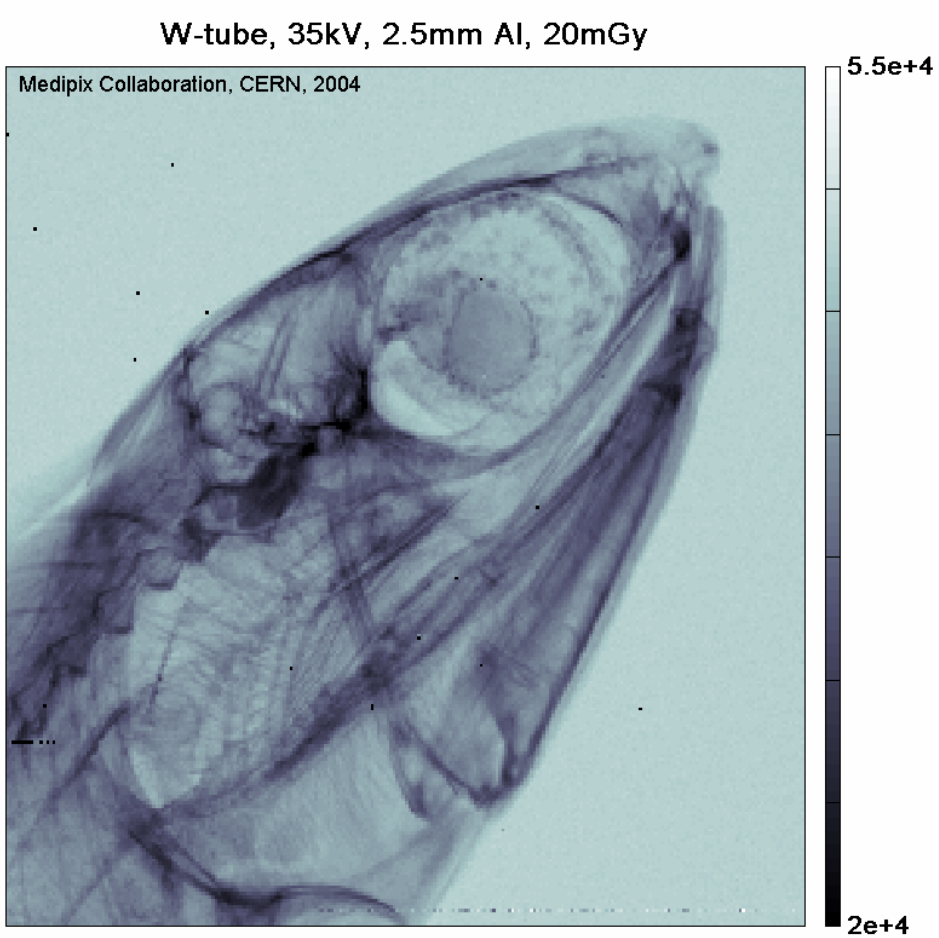

Image of a fly

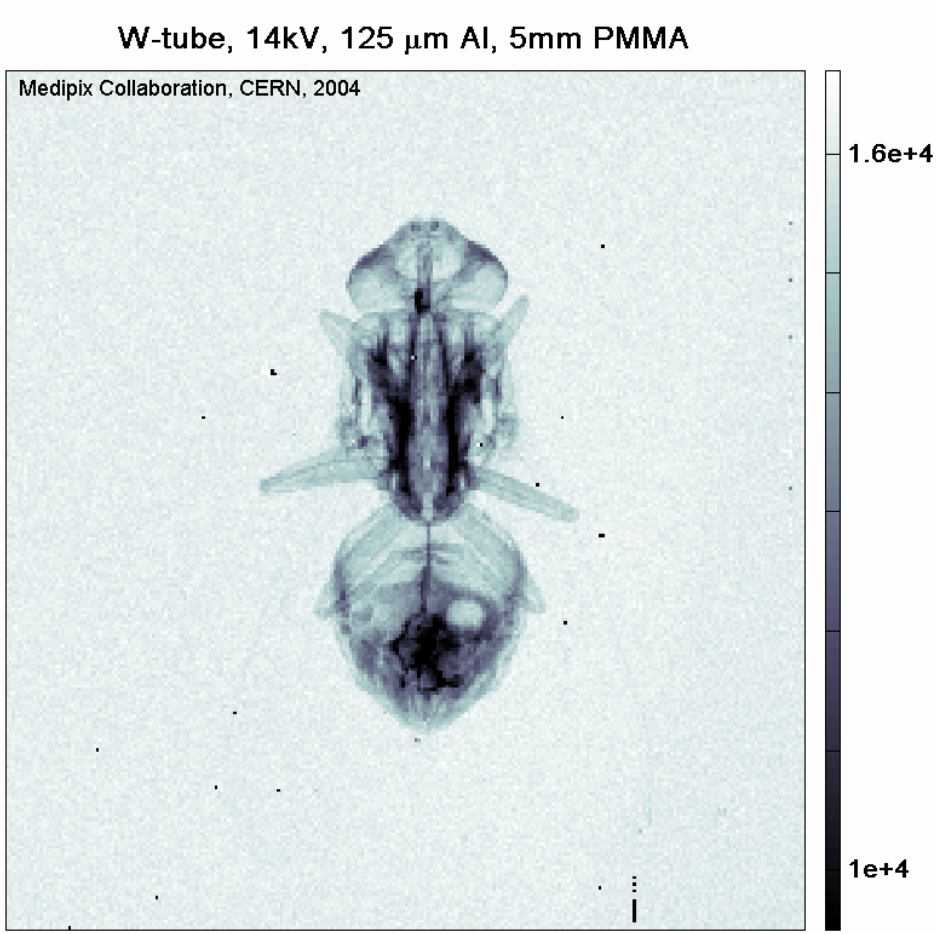

Image of a leaf (^{55}Fe)

Image taken over 14 Hours (5.9 KeV e^-)

Note celophane tape used to hold leaf in place…

And air bubble Surrounding leaf…

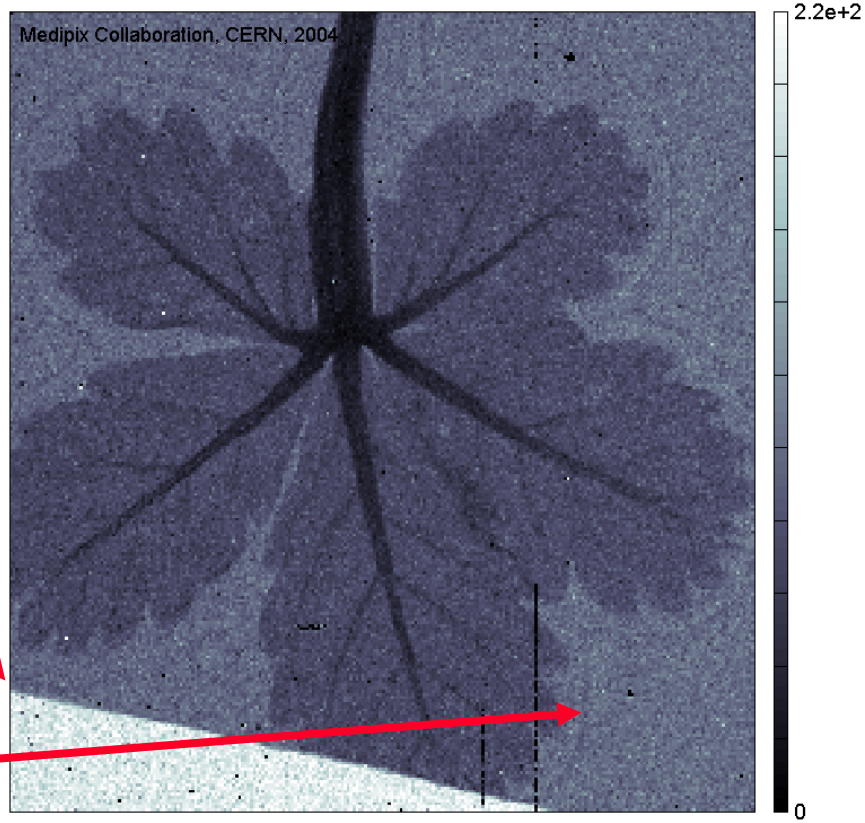

High rate images

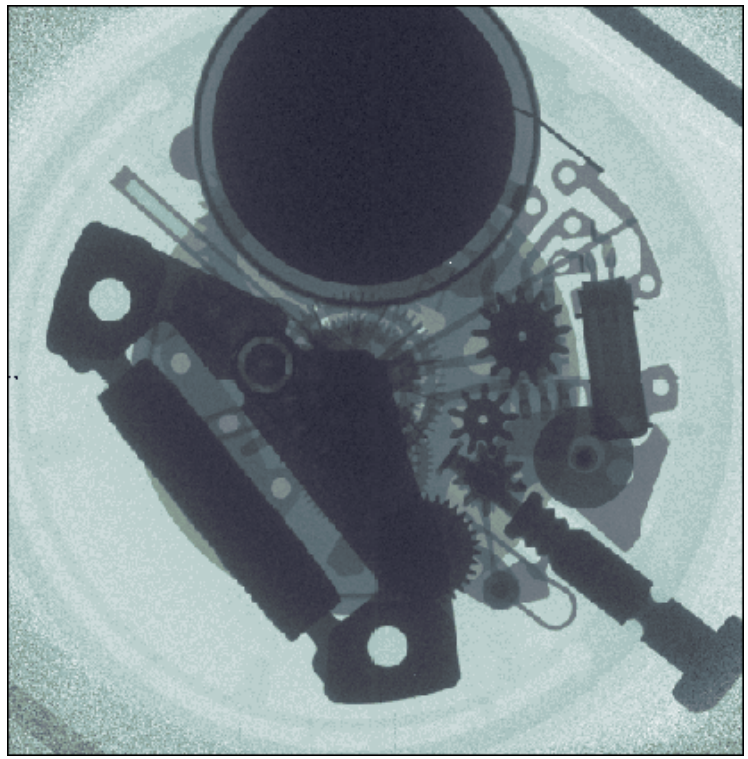

X-Ray movie at 5.5fps 512x512 pixels
Uses 4-chip Quad detector

Neutronography & Neutron Dosimetry

Lukas Tlustos, Czech Technical University, Prague *(To be developed by the University of Houston)*

- **Detection of light elements due to different attenuation of neutrons in matter, strong attenuation by H -> organic materials**
- **Conversion of thermal neutrons to heavy charged particles in ^{6}Li converter layer**
- **Reaction: $^{6}Li + n \rightarrow \alpha$ (2.05 MeV) + ^{3}H (2.72 MeV) Cross section: 940 barns (0.0253 eV)**

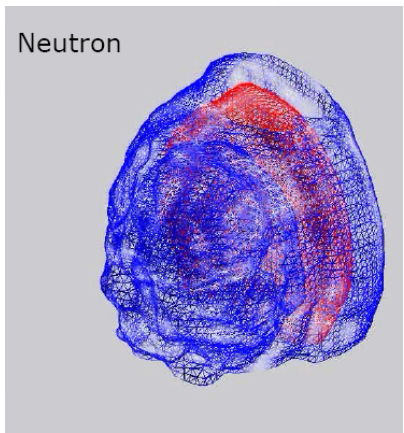

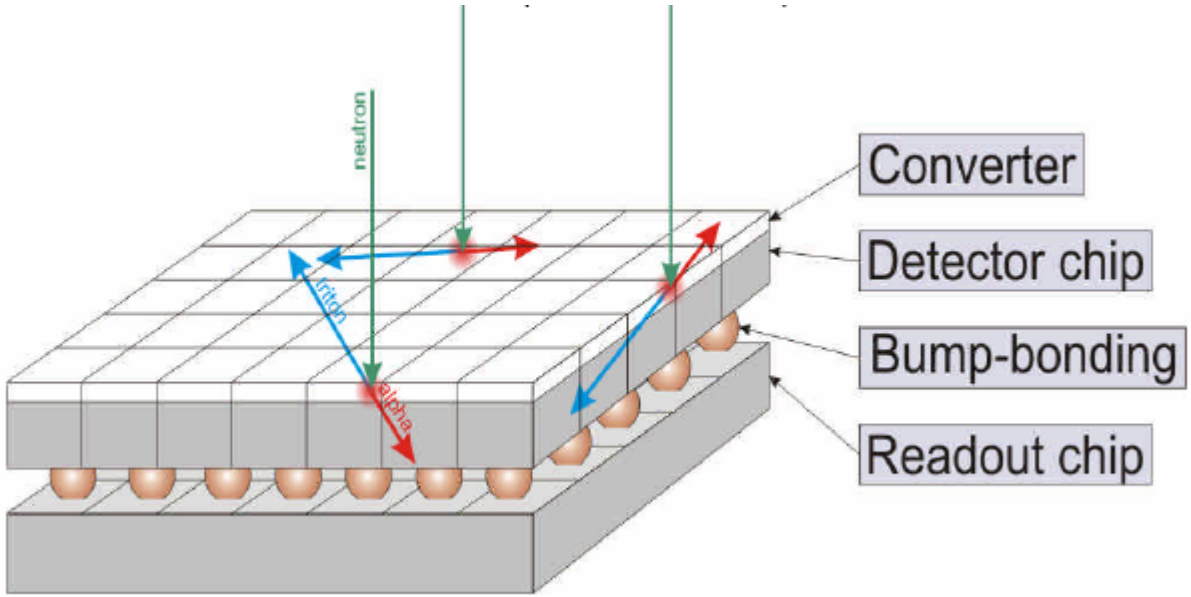

Monte-Carlo efficiency simulations

Detection efficiency was simulated in dependence on the converter thickness

- The neutron transport simulated using MCNP
- Energy deposition and ionization computed by TRIM/SRIM

940 barns (0.0253 eV)

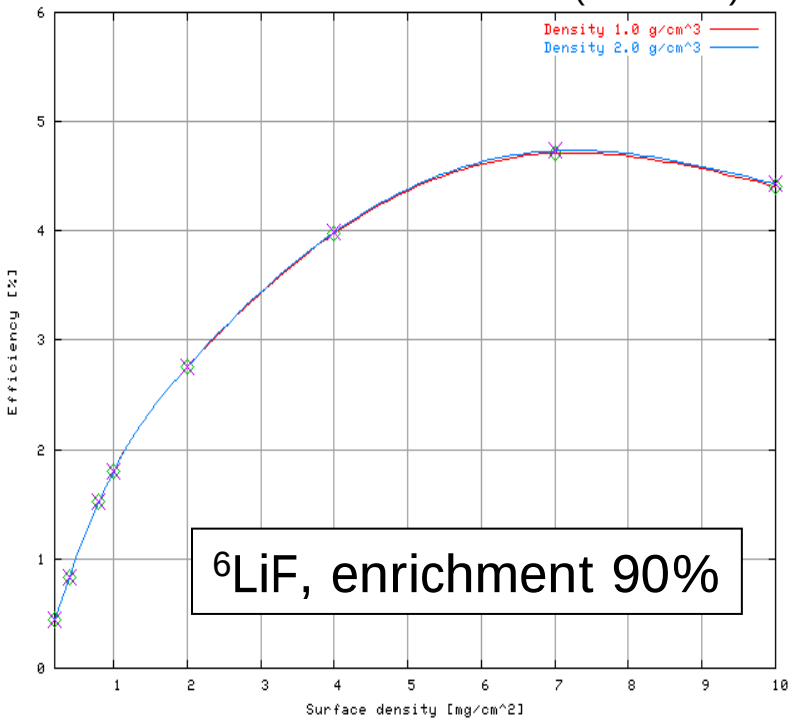

^{6}LiF, enrichment 90%

3840 barns (0.0253 eV)

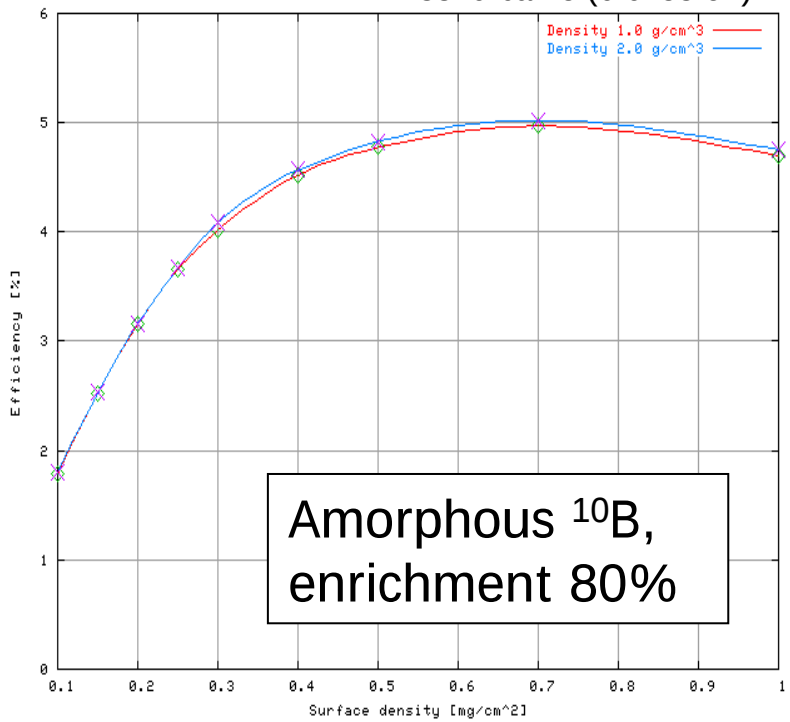

Amorphous ^{10}B, enrichment 80%

Spatial resolution estimation

Spatial resolution is affected by:

- Range of heavy charged particles in converter material – depends on density
  ^{6}LiF (ρ=1.6 g/cm^3): R_{Triton}=52μm, R_{α}=10μm
  ^{10}B (r=1.2 g/cm^3): R_{Li}=5μm, R_{α}=7μm
- Range in silicon
  ^{6}LiF: R_{Triton}=44.1μm, R_{α}=8.6μm.
  ^{10}B: R_{Li}=3μm / 2.7μm, R_{α}=5.4μm / 5.2μm
- Charge sharing effect ?

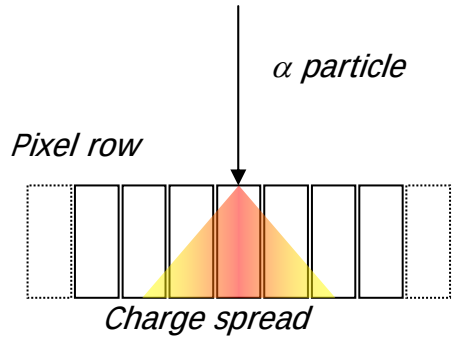

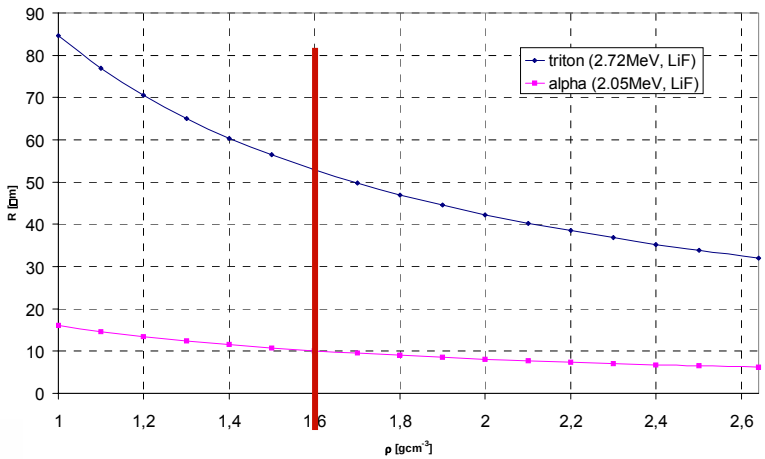

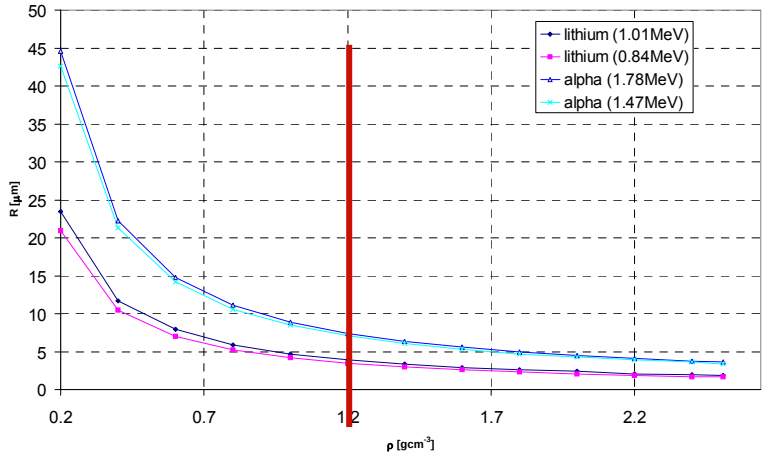

^{6}LiF converter

- Sensor covered by ^{6}LiF layer (3mg/cm^{2}). Detection efficiency is about 3%.
- High energy of alpha particles and tritons is deposited near detector surface => charge sharing is significant.

- Each hit creates signal in cluster of pixels.
- Cluster size limits spatial resolution in integrating regime.
- Cluster size can be decreased by high threshold at the expense of efficiency.

- Using event-by-event acquisition and finding centroids of clusters it is possible to reach subpixel spatial resolution (approximately half of pixel)

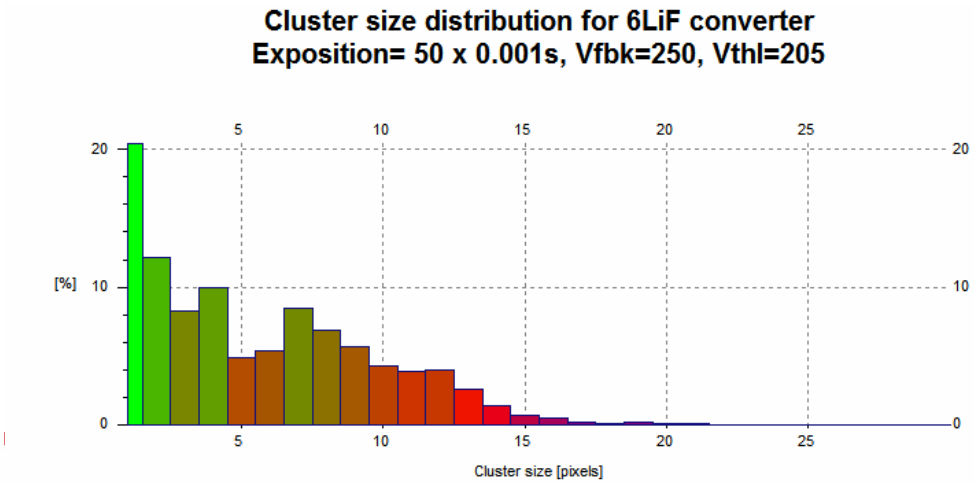

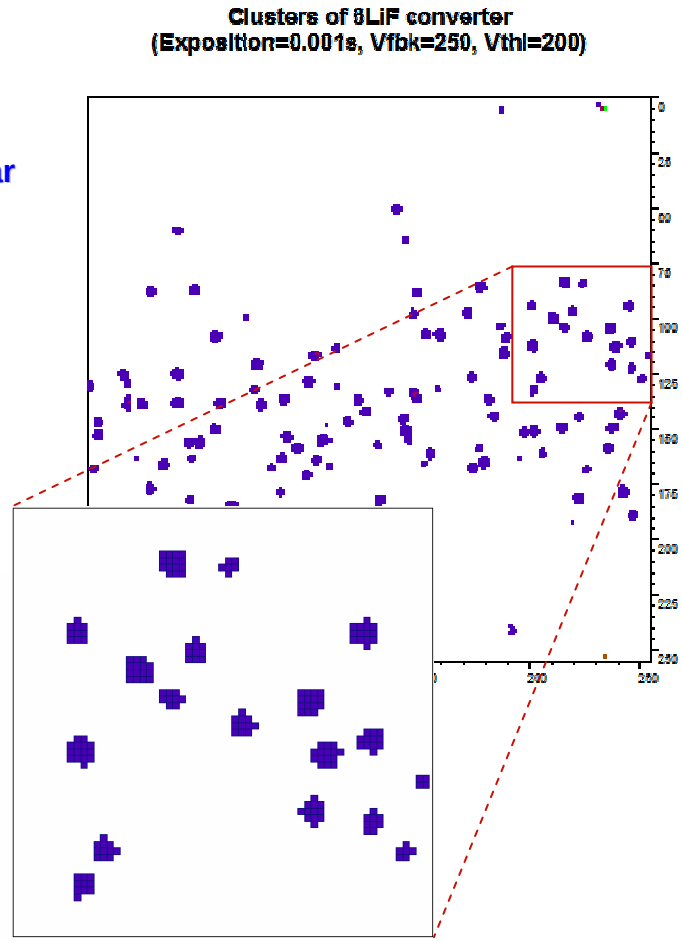

Amorphous ^{10}B converter

- Energy of heavy charged particles is lower than in case of ^{6}Li converter => smaller clusters are produced.
- From γ interactions electrons are generated => electron tracks are present. Spatial resolution is deteriorated by electron tracks.
- Energy of electrons is lower then energy of heavy particles => electron tracks can be suppressed by suitable threshold selection.

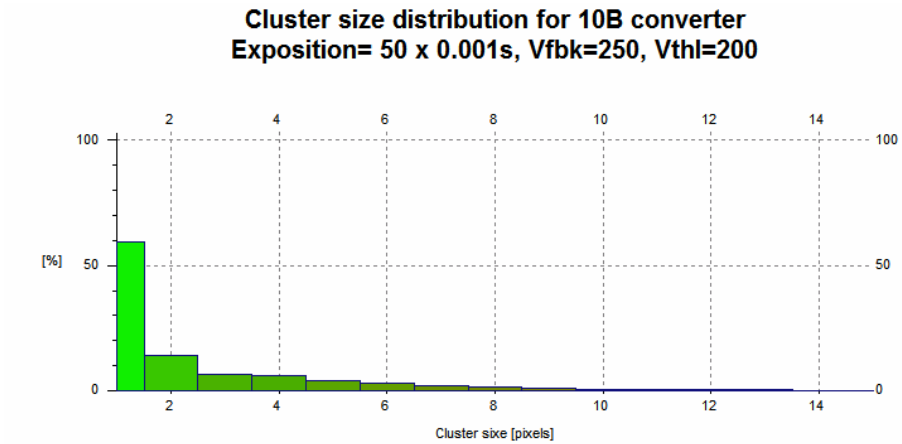

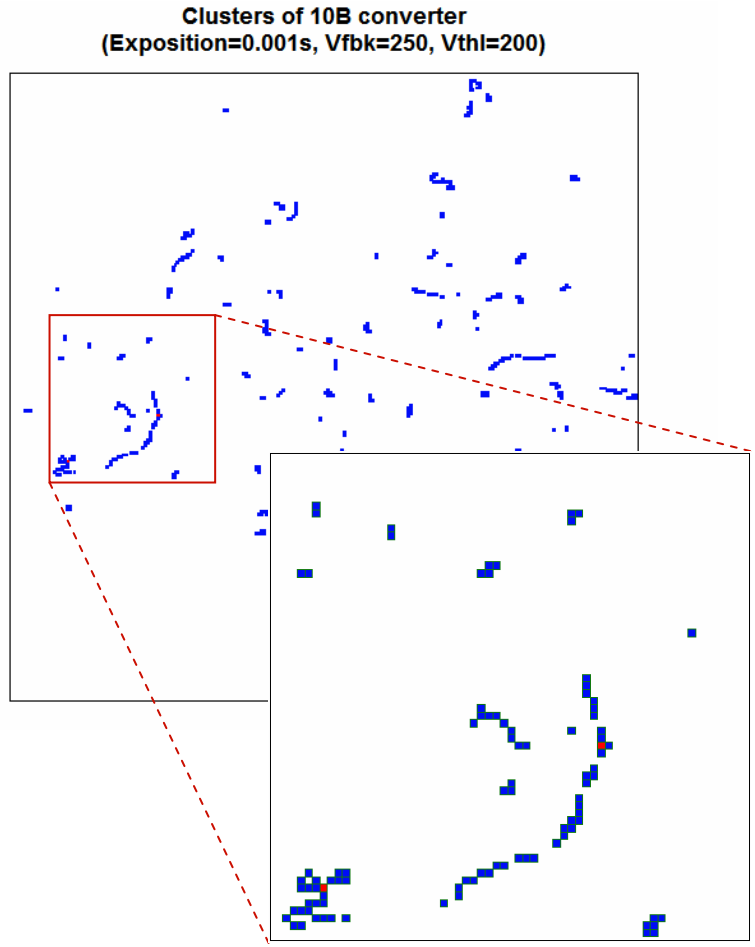

Recent Heavy Ion Measurements with Medipix2 (@ HIMAC & TAMU)

- **In collaboration with Jack Miller's Group at LBL, and Eric Benton, we recently made measurements with a Medipix2 of tracks in beams of:**
  - **Fe @ 500 Mev/A**
  - **O @ 290 MeV/A**
  - **Si @ 800 MeV/A**
  - **Ne @ 390 MeV/A**
- **This past weekend, in collaboration with NASA/JSC/SRAG, measurements were made at Texas A&M's cyclotron in beams of:**
  - **Xe @ 12 & 24 MeV/A**
  - **p @ 20, 30 & 40 MeV**

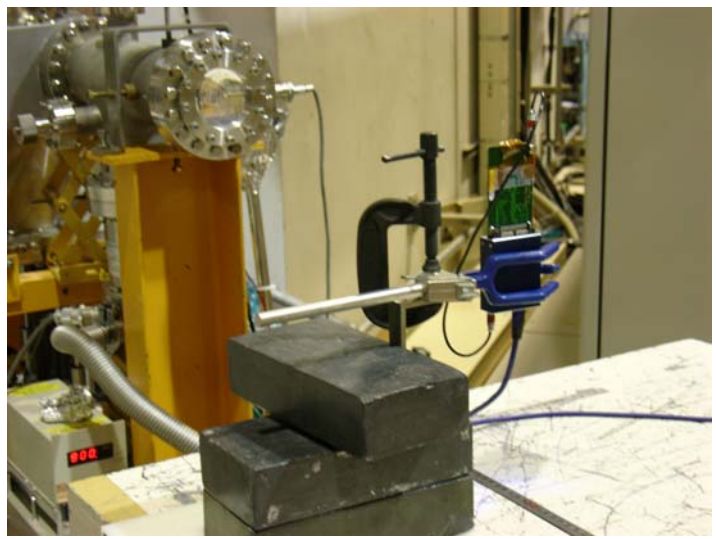

Heavy Ion Images in Medipix2

- **Pixels indicate above lower threshold & below upper threshold…**
- **These are effectively the energy slices through the track structure…**

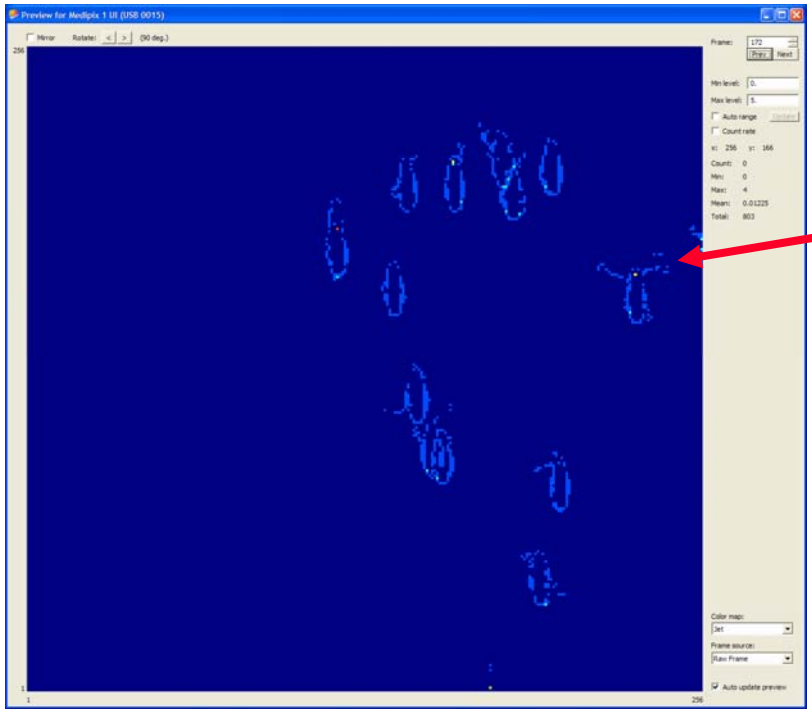

Note: δ-rays

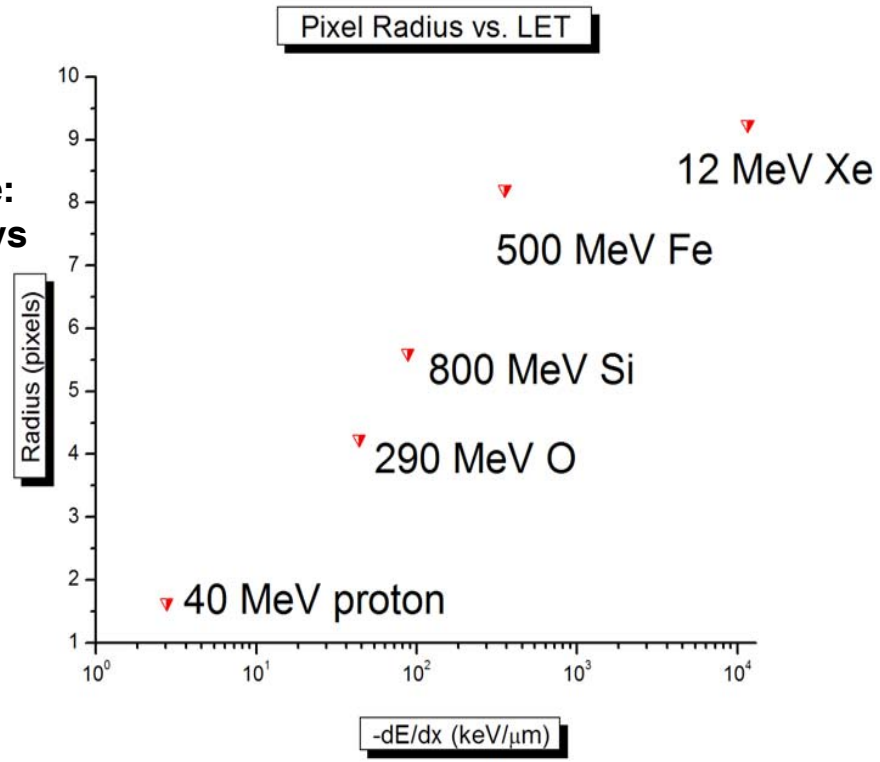

60 Degree Incidence O @ 290 MeV/A

Image Slice Size v. LET for beams taken

Medipix Movie of Xe Beam from This Past Weekend at A& M Cyclotron



100 Sec Integrated Medipix2 Images

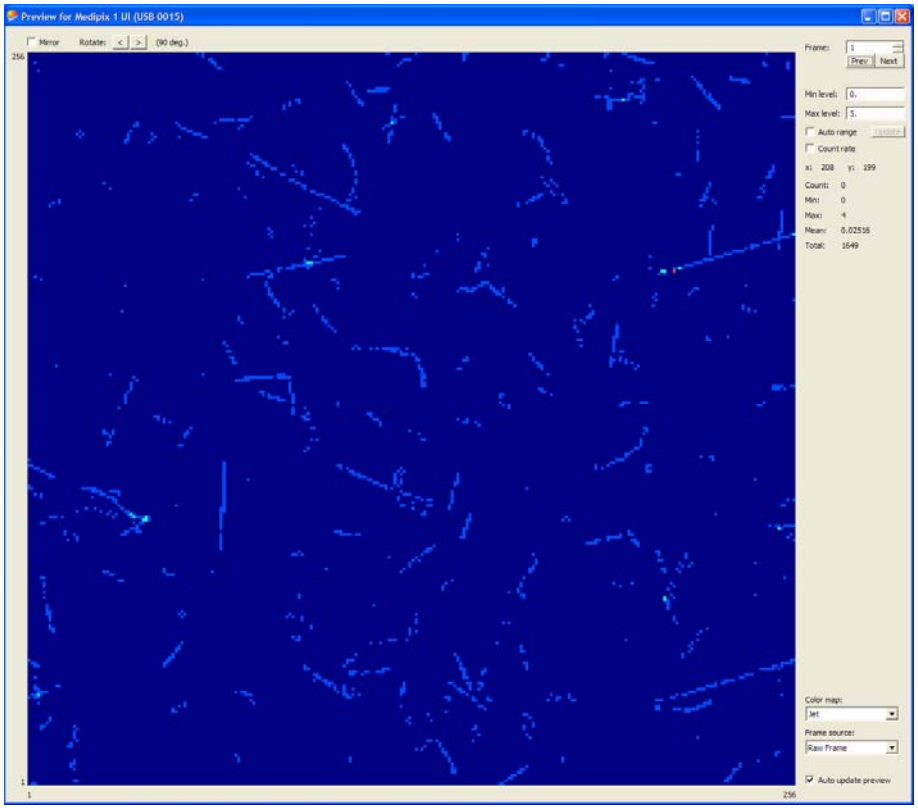

On my lap in a 777 airliner at 34,000 Feet over Anchorage, Alaska on the flight to Japan…

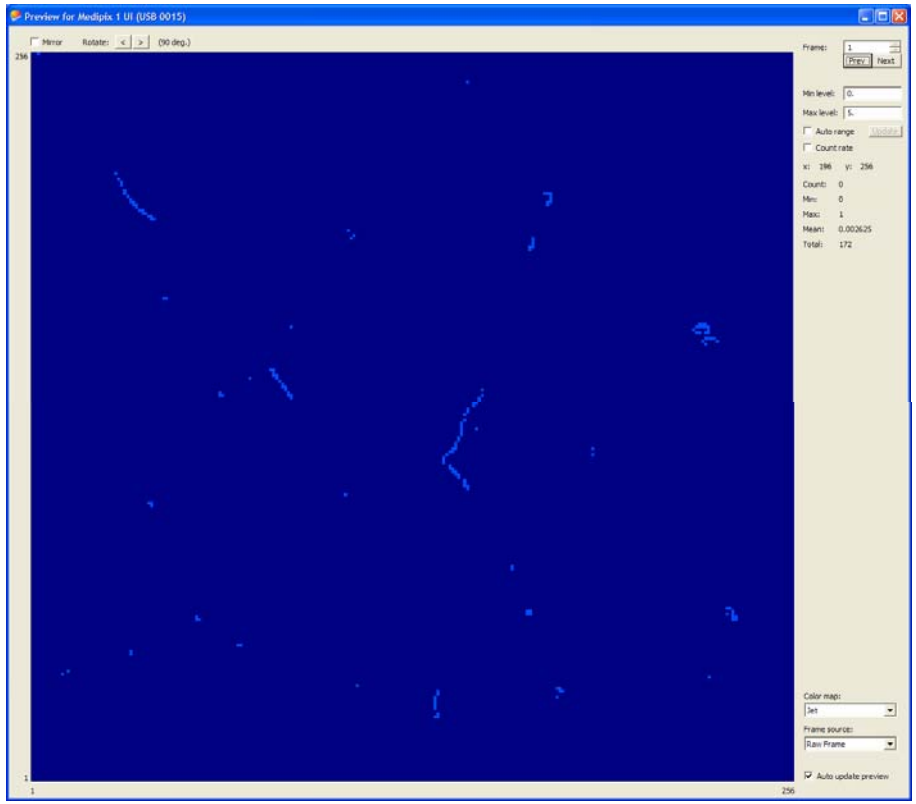

On the 15th floor of the Mitsui Garden Hotel in Chiba, Japan…

α Source

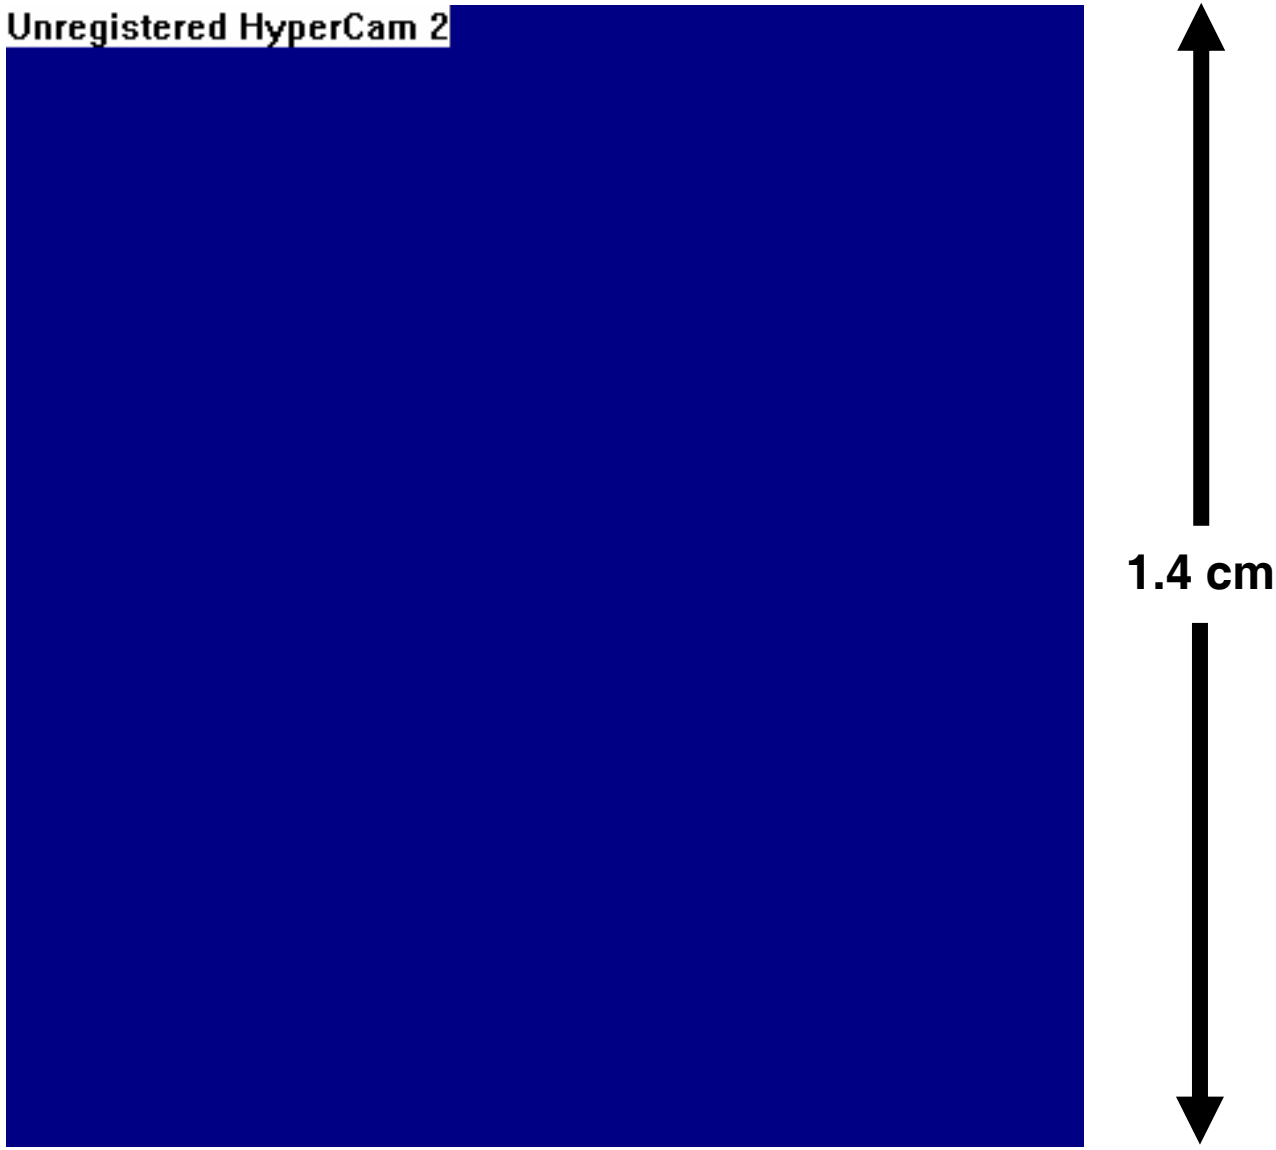

Adding Pulse Height Capability…
Timepix Schematic
for next the version of Medipix2

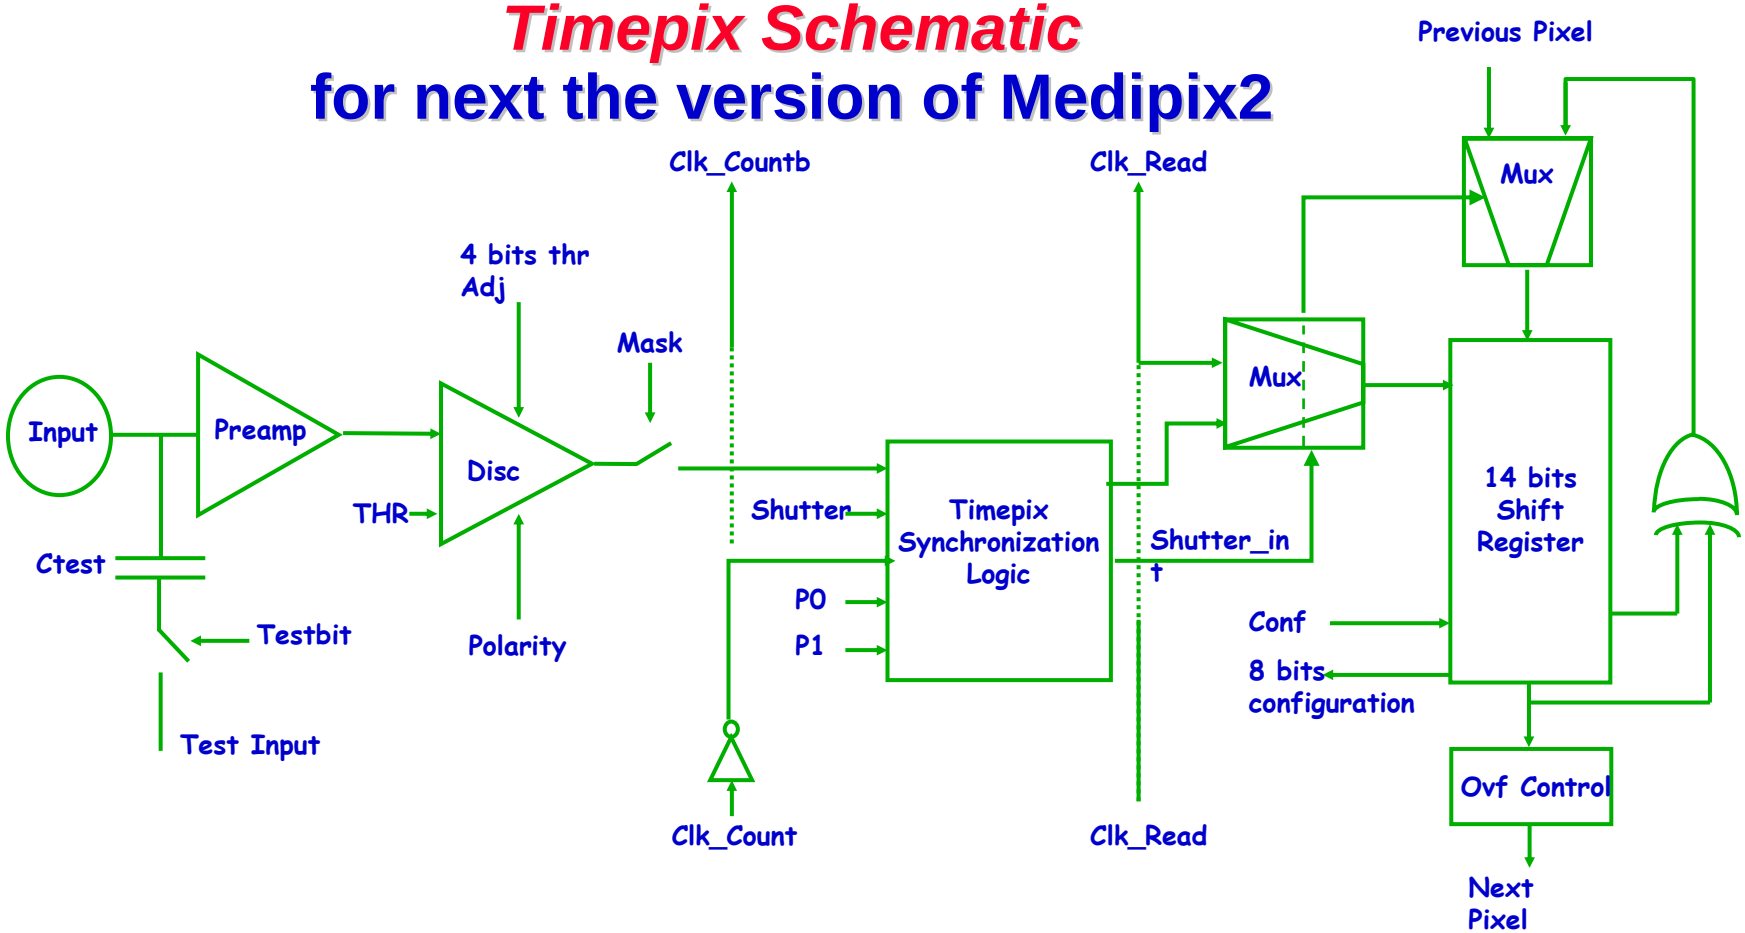

Analog

Digital

Analog pixel summary

Amplifier Gain	~18mV/Ke	
Peaking Time	90ns…140ns (IPreamp)	
Pixel noise	~75e^-_{rms}	
Preamp DC Level (FBK)	800mV (e^-)	1.4V (h^+)
Threshold dispersion	~170e^-	
Adjusted Threshold dispersion	~25e^-	
Voltage linear range	0 to 50 Ke^- (< 2%)	
TOT linear range	>200Ke^-	
Time Walk	~25ns (2Qth to ∞)	
TOTgain	~55ns/Ke^- (Ikrum=5nA)	
Analog Pixel consumption (Max)	2.9µA x 2.2V = 6.38 µW (30% less than Mpix2MXR20)	

All these values are extracted from simulations !!!

Timepix Synchronization Logic control

- Use of 3-bit High threshold adjustment bits for : 4th equalization bit and P0, P1.
- Each pixel can be configured independently in 5 different modes.
- This logic needs 104 Trts (Mpix2MXR20 had 92 Trts)
- Logic only consumes power only when a hit is present

Mask	P1	P0	Mode
0	0	0	Masked
0	0	1	Masked
0	1	0	Masked
0	1	1	Masked
1	0	0	Medipix
1	0	1	TOT
1	1	0	Timepix-1hit
1	1	1	Timepix

Timepix Mode (P0=1,P1=1)

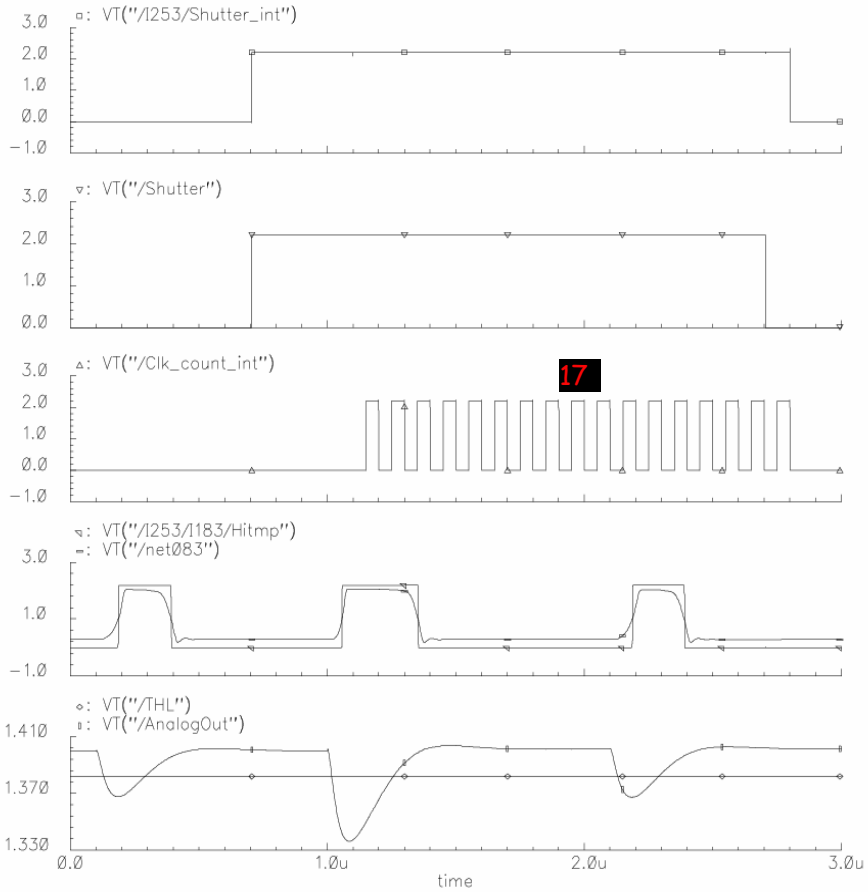

10MHz

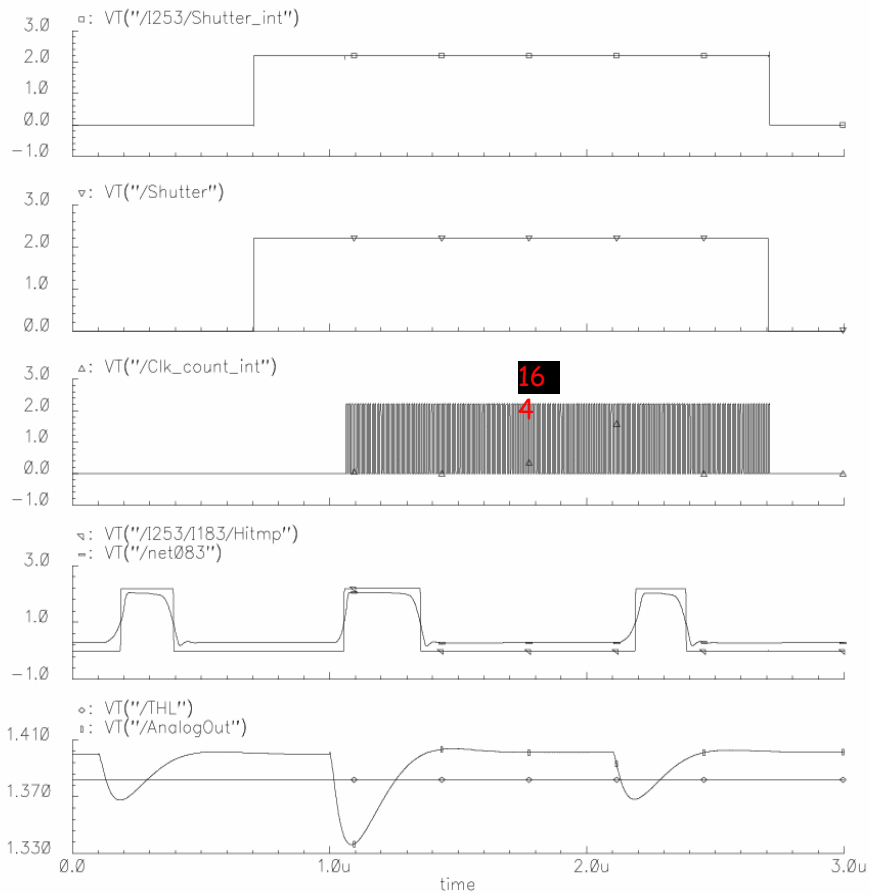

100MHz

TOT Mode (P0=1,P1=0)

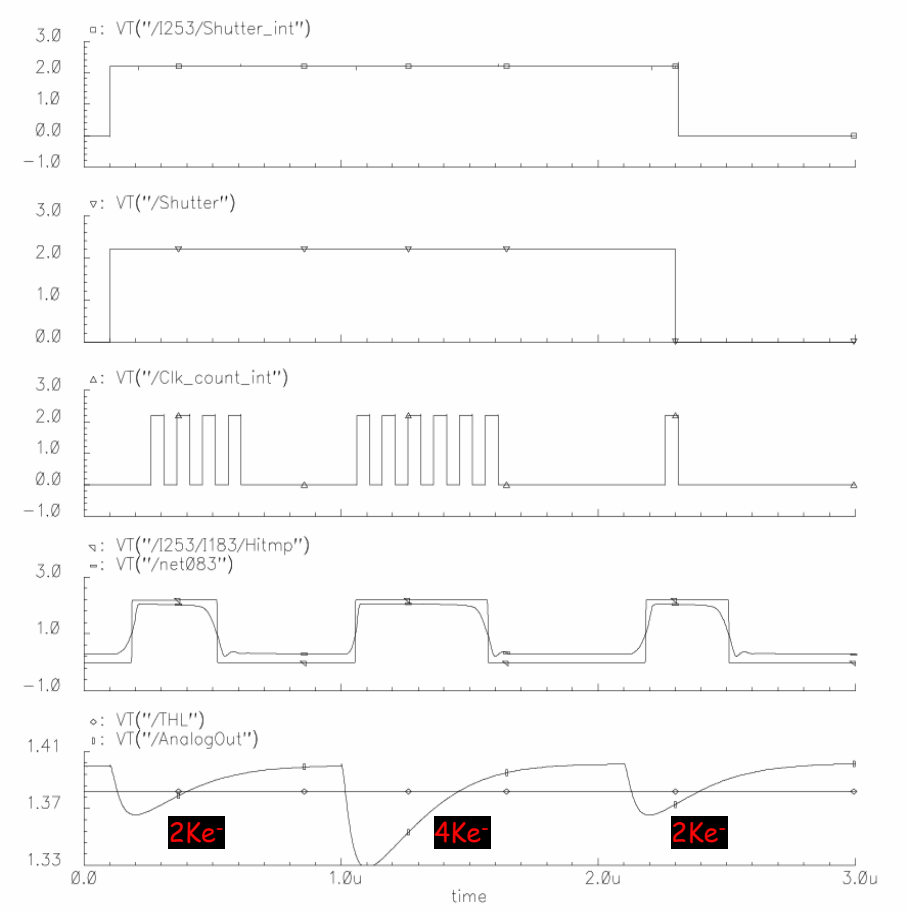

10MHz

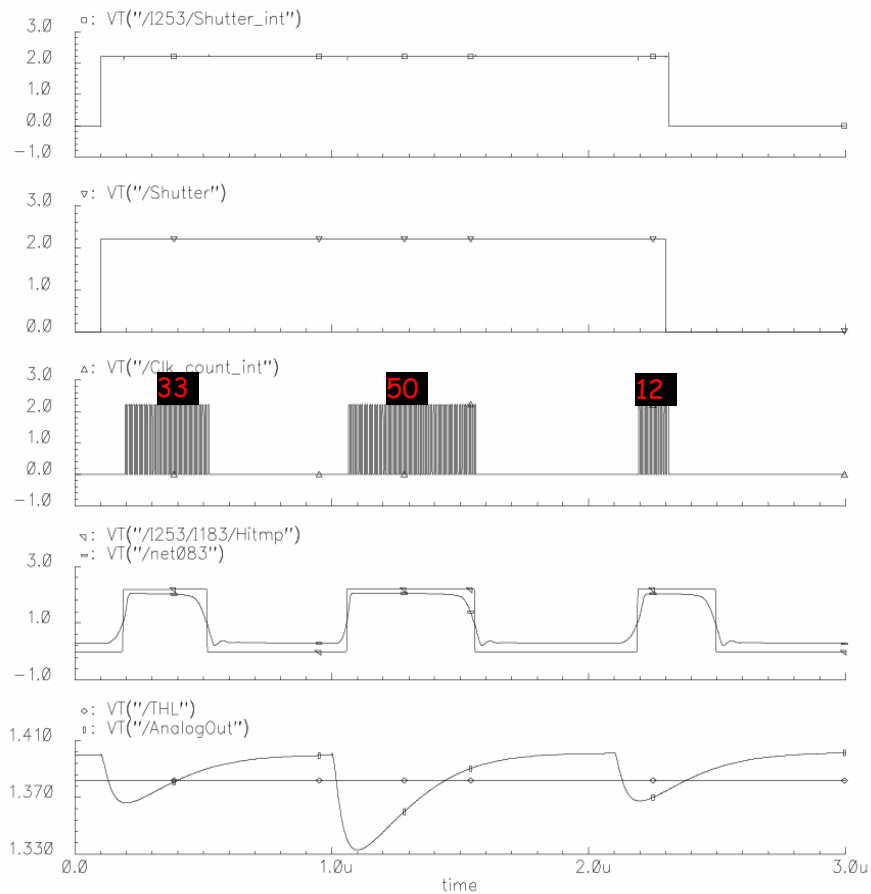

100MHz

Timepix proposed Floorplan

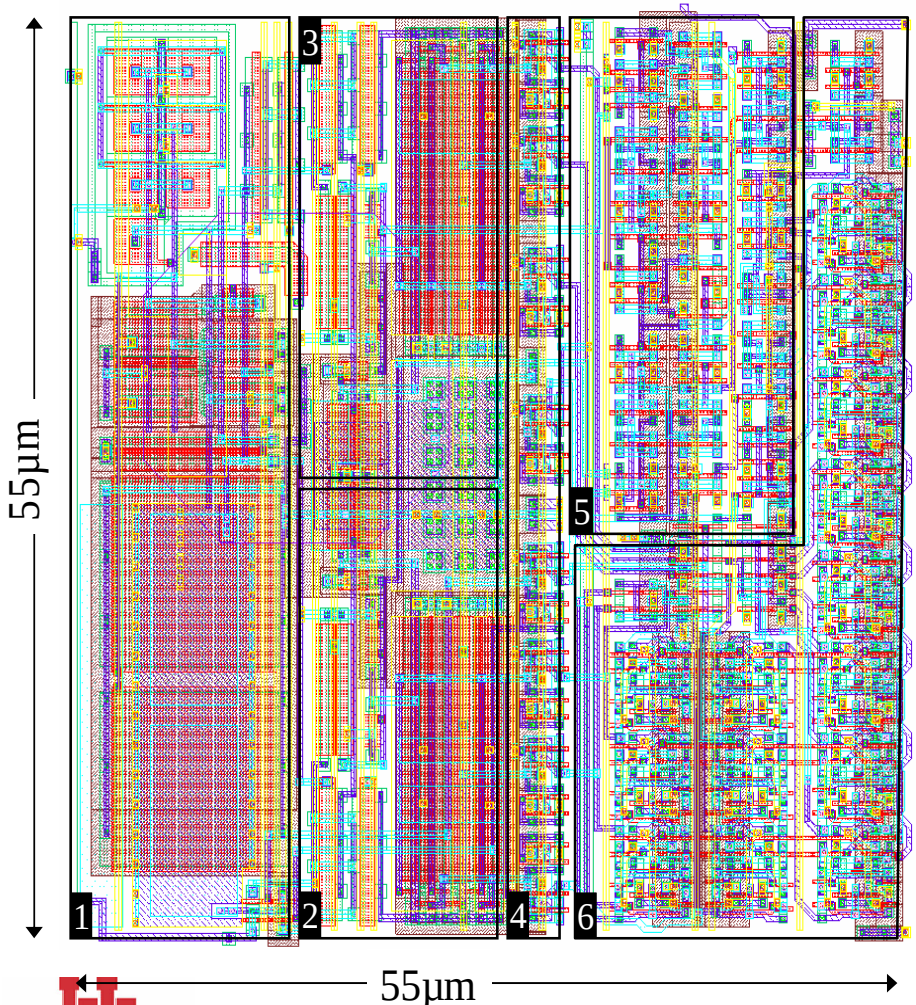

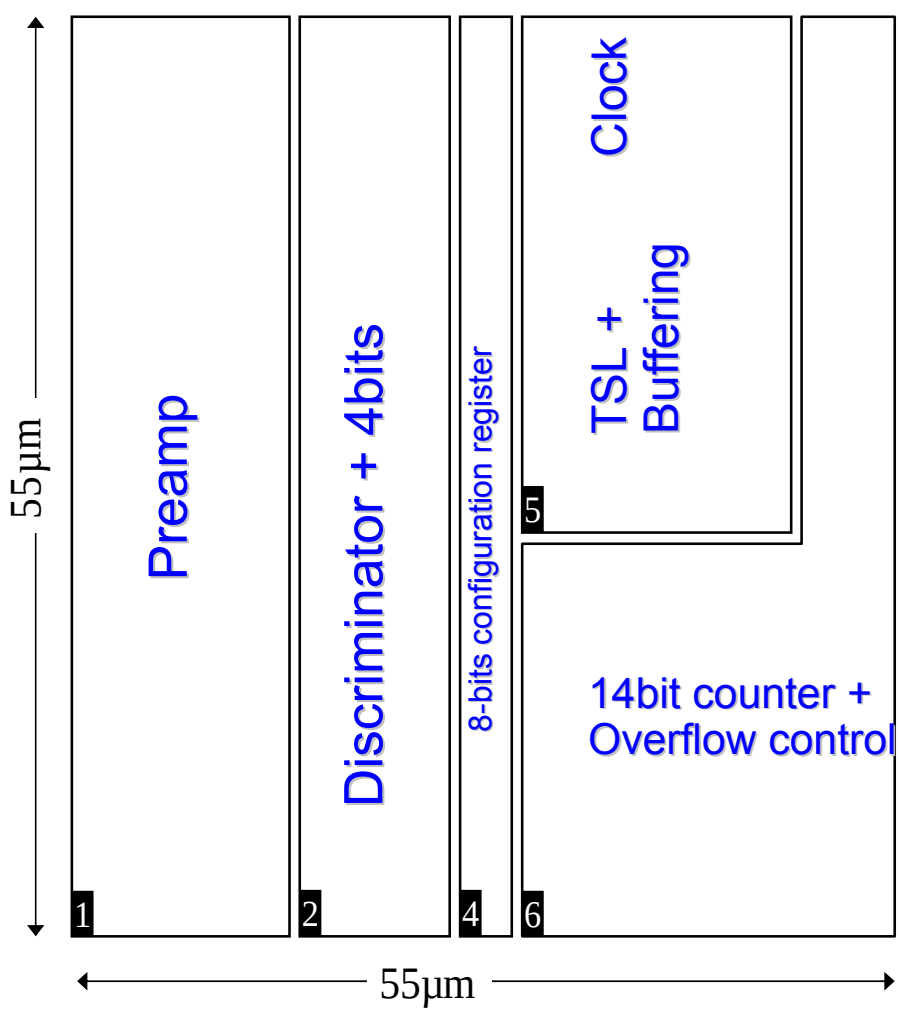

Mpix2MXR20 layout

Timepix proposed floorplan

Timepix - Summary

- Timepix development is driven by TPC readout for the ILC (EUDET consortium)
- Timepix will act as proof of principle for concept using existing Medixix2 readout system and software
- Initially foreseen for Time of Flight, the chip is now programable to measure Time over Threshold…
- Chip design is in final stages
- Submission planned end of May, 2006

Medipix3 – The Next Generation

- New pixel electronics taking care of charge diffusion – event-by-event clustering
- Flexible architecture – 2 counters per pixel
- Higher acquisition and frame rate with dead time free readout possible
- Small prototype just in testing
- Uses 0.13μm CMOS
- Medipix3 will attempt to resolve many of the limitations of the Medipix2 system
- Collaboration agreement ready for signature
- Could be made Rad-Hard…

Comparison Medipix2/Medipix3 - Si

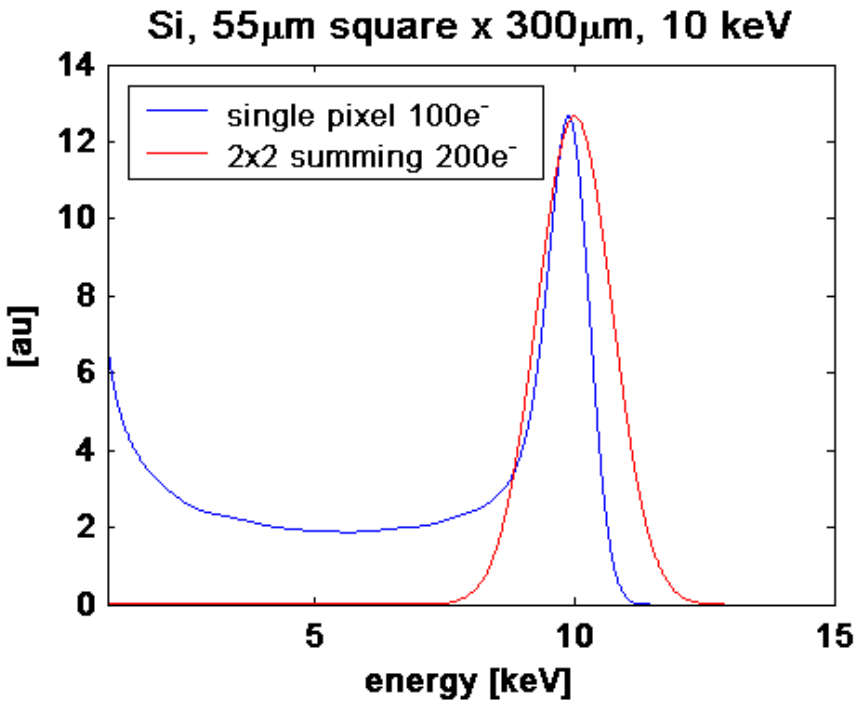

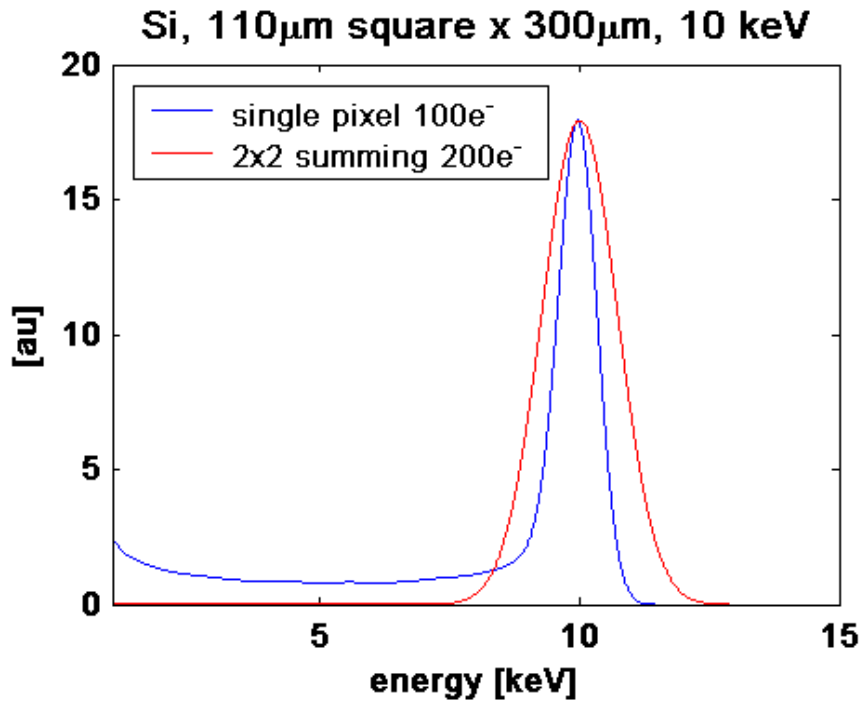

$\mu\tau \sim 5.8e3$ cm
Vbias = 120V

Where Do We Go From Here?

- The University of Houston would like to join the Medipix Consortium for the purpose of developing a Space Radiation Dosimeter based on the Medipix Technology. Funding from NASA is needed to initiate this effort.
- The imminent availability of the Timepix version of the Medipix2 chip offers an immediate opportunity to develop prototype flight hardware for evaluation.
- Longer term, we would like to also join the new Medipix3 Consortium to participate in the development of a robust versatile portable personal active Space Radiation Dosimeter…

Thank You For Your Attention..

Real-time demo to follow…

Time permitting

Medipix2 Chip Architecture

256 x 256 pixels

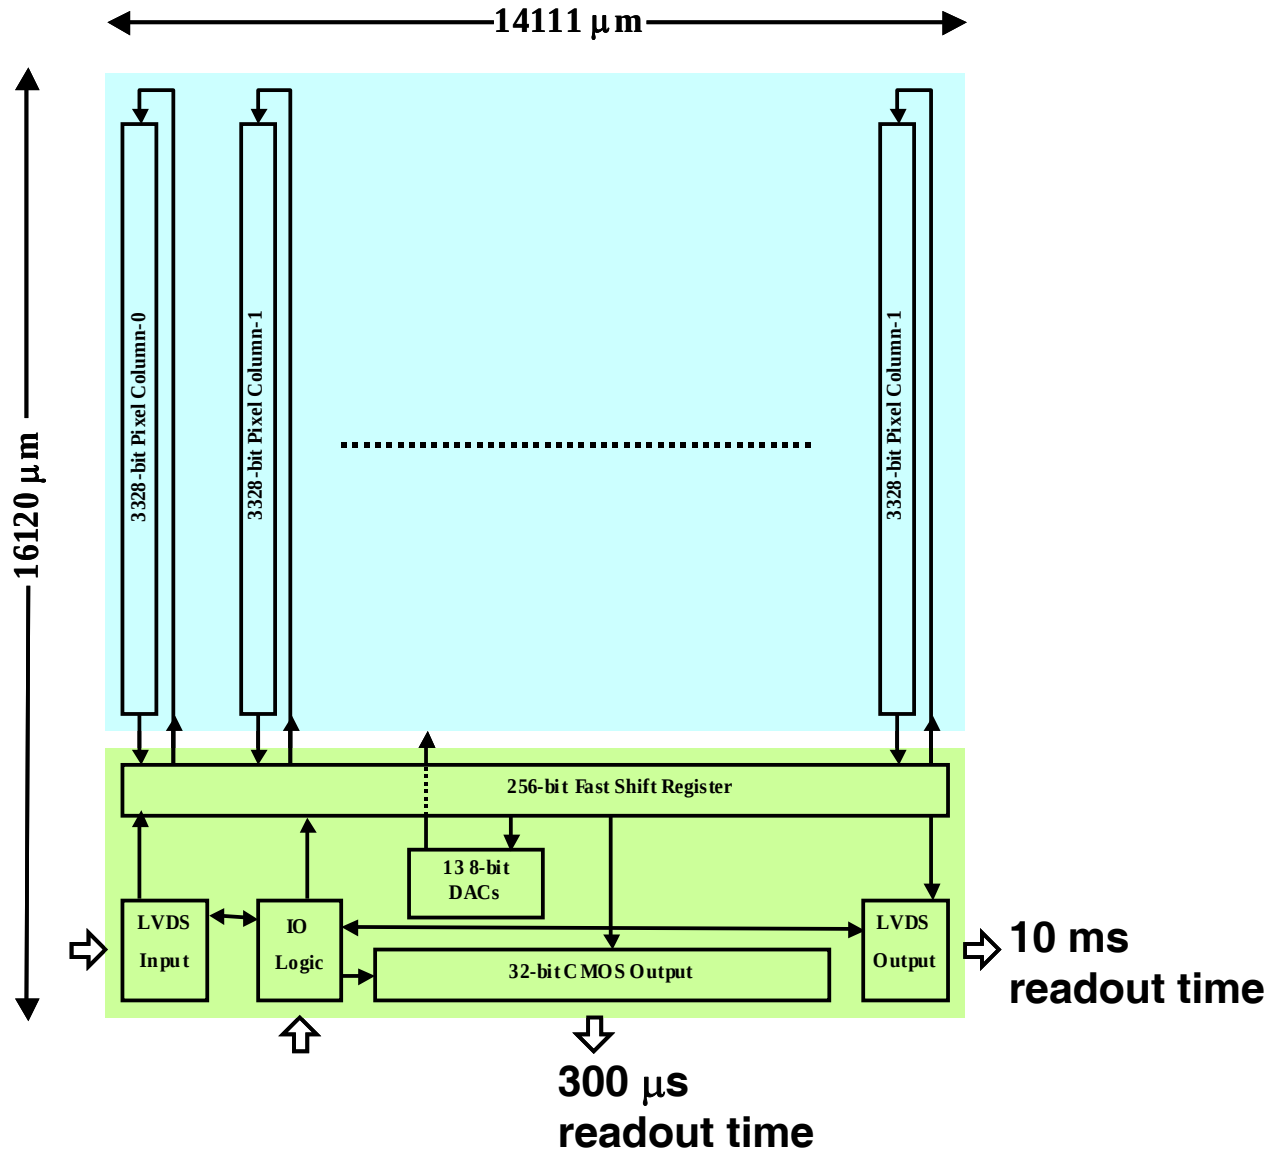

Tests of Medipix2 with alpha particles

- Medipix-2 without converter layer
- Alpha particles: 5.6 MeV (^{241}Am)
- Short exposition time
- Circular clusters observed

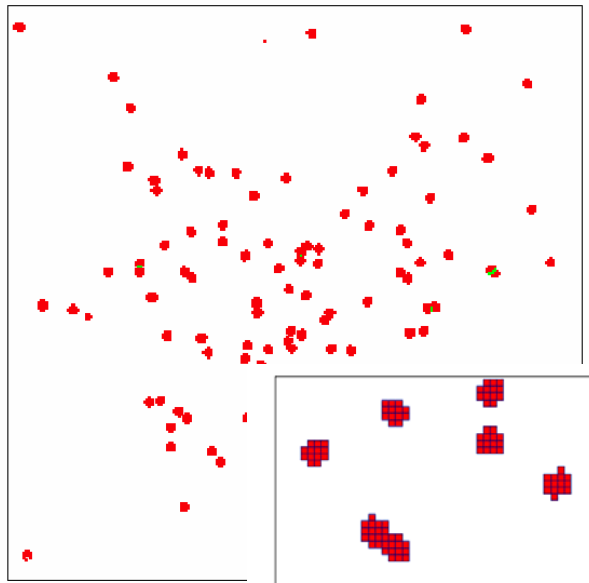

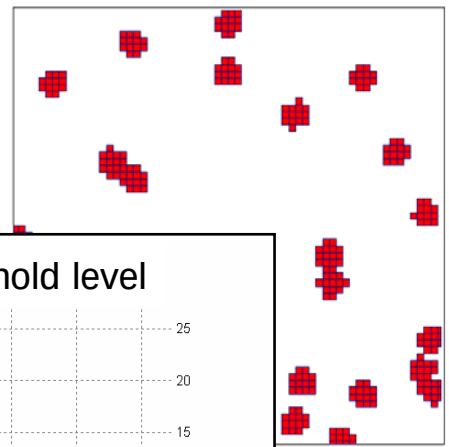

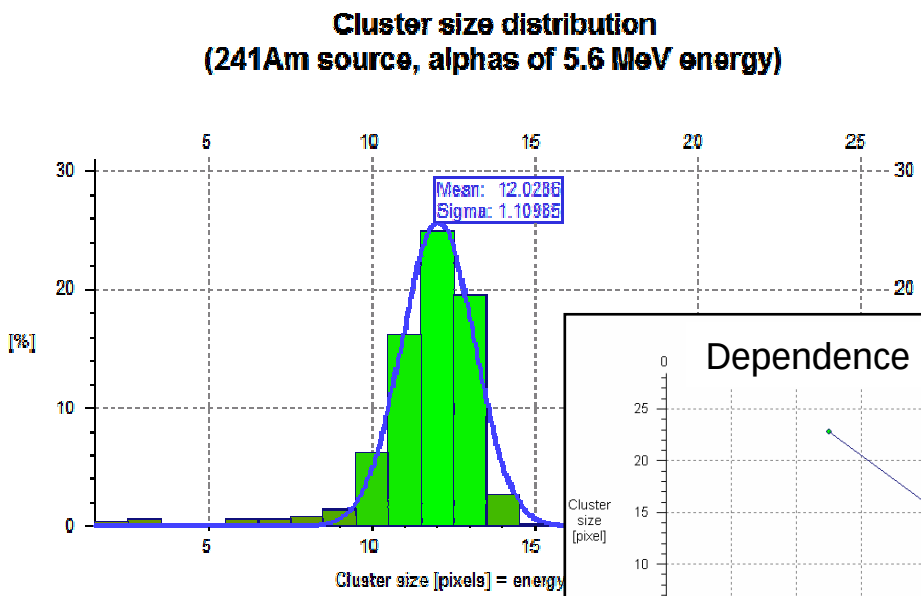

Tests with Thermal Neutrons

- **NEUTRA station of spallation neutron source SINQ in Paul Scherrer Institute, Villigen, Switzerland**
  - **Intensity about $3 \cdot 10^6$ neutrons/cm^{2}s at proton accelerator current of 1mA and proton energy of 590 MeV**
  - **Beam Cross section: 40 cm in diameter**
- **Horizontal channel of the LVR-15 nuclear research reactor at Nuclear Physics Institute of the Czech Academy of Sciences at Rez near Prague.**
  - **Intensity is about 10^7 neutrons/cm^{2}s (at reactor power of 8MW)**
  - **Beam Cross section: 4 mm (height) x 60 mm (width)**
  - **The divergence of the neutron beam is < 0.5°**

^{6}LiF converter
Spatial resolution – Edge response

Tilted cadmium edge profile

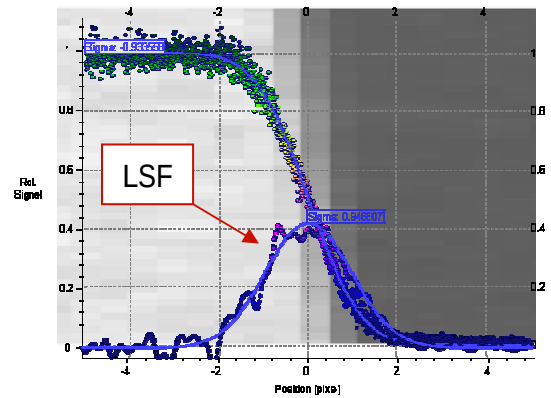

Fit by ERF: σ=0.83 pixel
=> LSF FWHM=107 μm

Edge blurring is caused by clusters => Spatial resolution is dependent on the threshold level

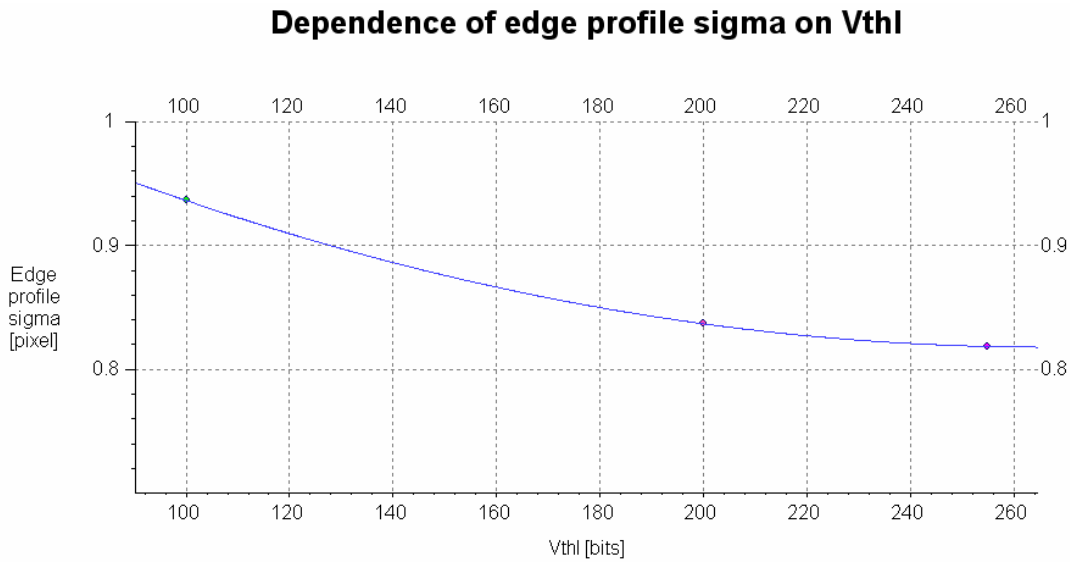

Spatial resolution is limited by size of clusters and range of product particles in silicon (R_{Triton}=44μm, R_{α}=8.9μm)

^{10}B converter
Spatial resolution – Edge response

Tilted cadmium edge profile

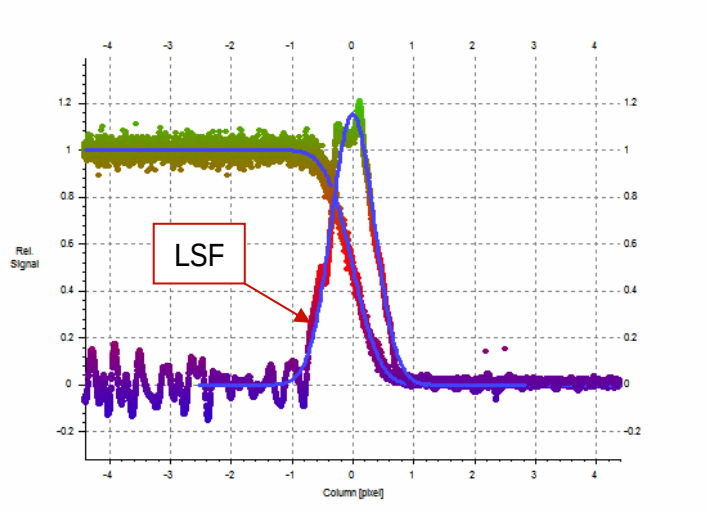

Fit by ERF: σ=0.35 pixel
=> LSF FWHM=45 μm

Heavy charged particles emitted by ^{10}B converter have shorter ranges then in case of ^{6}Li. Their energies are also lower so charge sharing is less important.

$\Rightarrow$ Spatial resolution is better

But lower number of particles can penetrate to depleted volume of the detector.

$\Rightarrow$ Efficiency is lower (approx. 2 times)

^{113}Cd converter

- **Only conversion electrons are usable for imaging.**
- **Resolution highly deteriorated**
- **Using event-by-event acquisition and robust track analyzing algorithm it is probably possible to increase resolution.**

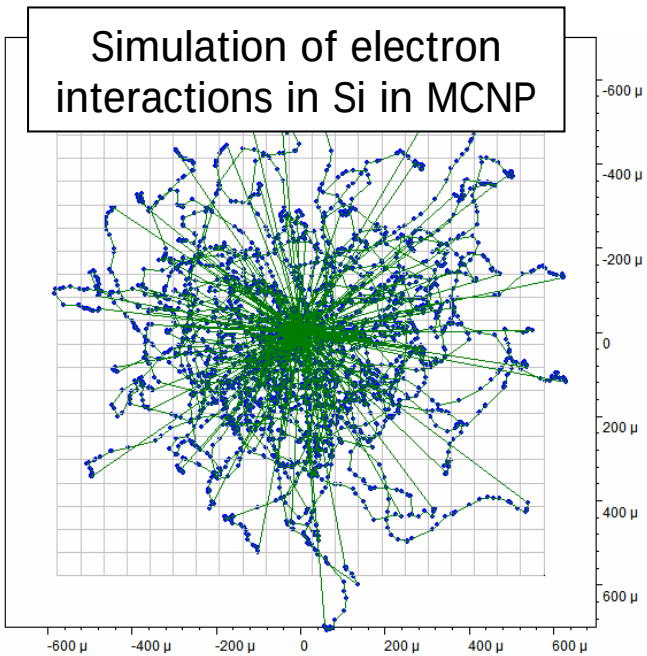

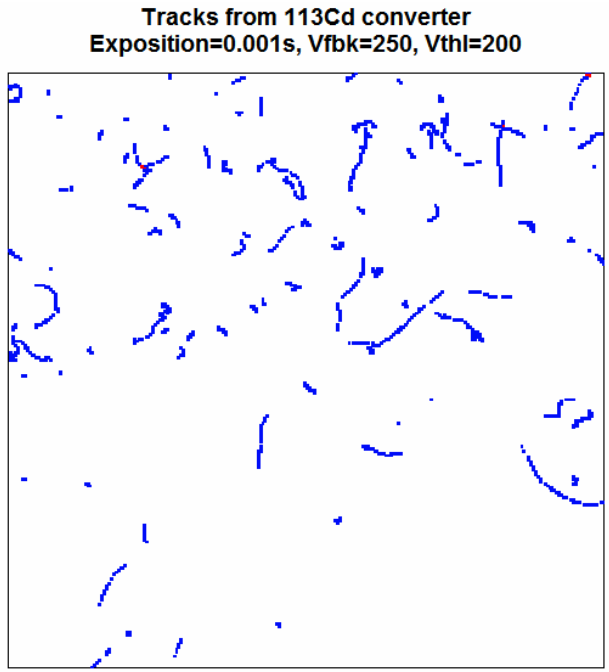

^{113}Cd converter
Spatial resolution – Edge response

Tilted cadmium edge profile

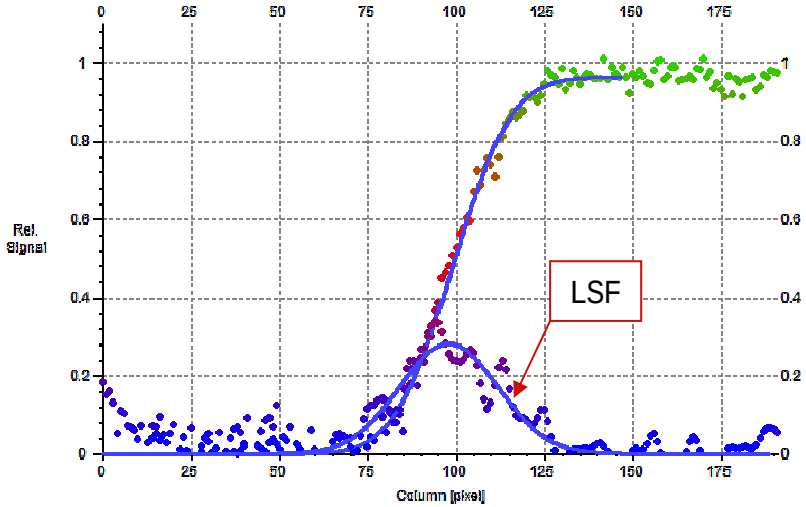

Fit by ERF: σ=13.1 pixel
=> LSF **FWHM=1.7 mm**

^{113}Cd as converter in combination with Si detector is not good choice for position sensitive detection of neutrons. But thanks to the large cross section it can reach good detection efficiency especially in case of **CdTe detectors**.

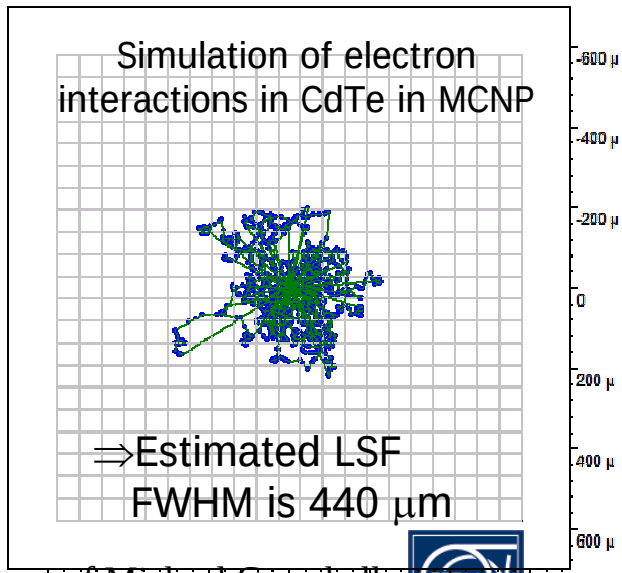

Slide Courtesy of Michael Campbell

Comparison of Medipix-2 with other neutron imaging detectors

Tested:

- **CCD camera** with scintilator containing ^{6}Li (pixel size 0.139 mm)
- **Imaging plate** (excitation by neutrons, deexcitation by laser scanner followed by light emission, scanner pixel size 50μm)
- **Medipix-1** device with ^{6}LiF converter
- **Medipix-2** device with ^{6}LiF converter

Imager	Resolution (FWHM[1] of LSF[2]) [μm]	Resolution[3] [lp/mm]
Medipix-1 device	370	2.5
Medipix-2 device	108	8.5
CCD camera	824	1.1
Imaging plate	124	7.3